



**GE Medical Systems**

---

# **Technical Publications**

**Direction 2142506–100**

**Revision 1**

## **Advantx DLX Dicom V3.0 (ID/NET V3.0) Conformance Statement**

**do not duplicate**

**Copyright © 1997 by General Electric Co.**



## TABLE OF CONTENTS

SECTION	TITLE	PAGE
	REVISION HISTORY .....	v
	LIST OF EFFECTIVE PAGES .....	v
<b>SECTION 1 – INTRODUCTION .....</b>		<b>1–1</b>
1–0	OVERVIEW .....	1–1
1–1	OVERALL Conformance Statement DOCUMENT STRUCTURE .....	1–1
1–2	INTENDED AUDIENCE .....	1–3
1–3	scope and field of application .....	1–4
1–4	important remarks .....	1–4
1–5	references .....	1–5
1–6	definitions .....	1–5
1–7	symbols and abbreviations .....	1–5
<b>SECTION 2 – CONFORMANCE STATEMENT .....</b>		<b>2–1</b>
2–0	introduction .....	2–1
2–1	IMPLEMENTation model .....	2–1
2–1–1	Application Data Flow Diagram .....	2–1
2–1–2	Functional Definition of AE’s .....	2–2
2–1–3	Sequencing of Real–World Activities .....	2–2
2–2	AE Specifications .....	2–2
2–2–1	AE Specification .....	2–2
2–2–1–1	Association Establishment Policies .....	2–3
2–2–1–1–1	General .....	2–3
2–2–1–1–2	Number of Associations .....	2–3
2–2–1–1–3	Asynchronous Nature .....	2–3
2–2–1–1–4	Implementation Identifying Information .....	2–3
2–2–1–2	Association Initiation Policy .....	2–3
2–2–1–2–1	Real–World Activity “Copy Image” .....	2–3
2–2–1–2–1–1	Associated Real–World Activity .....	2–3
2–2–1–2–1–2	Proposed Presentation Contexts .....	2–4
2–2–1–2–1–2–1	SOP Specific Conformance Statement for Image Storage SOP Class .....	2–4
2–2–1–2–2	Real–World Activity “Get Worklist” .....	2–5
2–2–1–2–2–1	Associated Real–World Activity .....	2–5
2–2–1–2–2–2	Proposed Presentation Contexts .....	2–5
2–2–1–2–2–2–1	SOP Specific Conformance Statement for Image Storage SOP Class .....	2–5
2–2–1–3	Association Acceptance Policy .....	2–6

2–2–1–3–1 Real–World Activity ”Verification acknowledge”	2–6
2–2–1–3–1–1 Associated Real–World Activity	2–6
2–2–1–3–1–2 Accepted Presentation Contexts	2–6
2–2–1–3–1–2–1 SOP Specific Conformance Statement for Verification SOP Class	2–6
2–3 Communication profiles	2–7
2–3–1 Supported Communication Stacks (parts 8,9)	2–7
2–3–2 TCP/IP Stack	2–7
2–3–2–1 API	2–7
2–3–2–2 Physical Media Support	2–7
2–3–3 Point–to–Point Stack	2–7
2–4 Extensions / specializations / privatizations	2–7
2–5 Configuration	2–7
2–5–1 AE Title/Presentation Address Mapping	2–7
2–5–2 Configurable Parameters	2–7
2–6 Support of extended character sets	2–7

**SECTION 3 XA INFORMATION OBJECT IMPLEMENTATION 3–1**

3–0 Introduction	3–1
3–1 XA Image IOD Implementation	3–1
3–2 XA Image IOD Entity–Relationship Model	3–1
3–2–1 Entities Description	3–2
3–2–2 DLX Mapping of DICOM entities	3–2
3–3 XA Image IOD Module Table	3–2
3–4 InFORMATION MODULE DEFINITIONS	3–3
3–4–1 Patient Entity Module	3–3
3–4–1–1 Patient Module	3–3
3–4–2 Study Entity Module	3–4
3–4–2–1 General Study	3–4
3–4–2–2 Patient Study	3–4
3–4–3 Series Entity Module	3–4
3–4–3–1 General Series	3–4
3–4–4 Equipment Entity Module	3–5
3–4–4–1 General Equipment	3–5
3–4–5 Image Entity Module	3–5
3–4–5–1 General Image	3–5
3–4–5–2 Image Pixel	3–6
3–4–5–3 Cine	3–6
3–4–5–4 Multi–Frame	3–6
3–4–5–5 Frame Pointers	3–6
3–4–5–6 Mask	3–7
3–4–5–7 Display Shutter	3–7

3-4-5-8 Device .....	3-7
3-4-5-9 X-Ray Image .....	3-8
3-4-5-10 X-Ray Acquisition .....	3-8
3-4-5-11 X-Ray Collimator .....	3-9
3-4-5-12 X-Ray table .....	3-9
3-4-5-13 XA Positioner .....	3-9
3-4-5-14 Curve .....	3-10
3-4-5-15 SOP Common .....	3-10
3-5 PRIVATE DATA DICTIONARY .....	3-11

**SECTION 4 – SECONDARY CAPTURE IMPLEMENTATION ..... 4-1**

4-0 Introduction .....	4-1
4-1 SC Image IOD Implementation .....	4-1
4-2 SC Image IOD Entity–Relationship Model .....	4-1
4-2-1 Entities Description .....	4-2
4-2-2 DLX Mapping of DICOM entities .....	4-3
4-3 SC Image IOD Module Table .....	4-3
4-4 Module Library .....	4-3
4-4-1 Patient Entity Module .....	4-4
4-4-1-1 Patient Module .....	4-4
4-4-2 Study Entity Module .....	4-4
4-4-2-1 General Study .....	4-4
4-4-2-2 Patient Study .....	4-4
4-4-3 Series Entity Module .....	4-4
4-4-3-1 General Series .....	4-4
4-4-4 Equipment Entity Module .....	4-5
4-4-4-1 SC Equipment Module .....	4-5
4-4-5 Image Entity Module .....	4-5
4-4-5-1 General Image .....	4-5
4-4-5-2 Image Pixel .....	4-5
4-4-5-3 Overlay Plane Module .....	4-6
4-4-5-4 SOP Common .....	4-6
4-5 PRIVATE DATA DICTIONARY FOR SECONDARY CAPTURE .....	4-6

**SECTION 5 – BASIC WORKLIST MANAGEMENT IMPLEMENTATION ..... 5-1**

5-0 INTRODUCTION .....	5-1
5-1 WORKLIST INFORMATION MODEL IMPLEMENTATION .....	5-1
5-2 WORKLIST INFORMATION MODEL ENTITY – RELATIONSHIP DIAGRAM ..	5-1
5-2-1 Entities Description .....	5-2
5-3 Basic Worklist Information Module Table .....	5-2
5-4 INFORMATION MODULE DEFINITIONS .....	5-2

5-4-1 Patient Entity Module .....	5-3
5-4-1-1 Patient Identification Module .....	5-3
5-4-1-2 Patient Demographic Module .....	5-3
5-4-1-3 Patient Medical Module .....	5-3
5-4-2 Visit/Facility Episode Entity Module .....	5-3
5-4-2-1 Visit Identification Module .....	5-3
5-4-2-2 Visit Status Module .....	5-3
5-4-2-3 Visit Relationship Module .....	5-3
5-4-3 Imaging Service Request Entity Module .....	5-4
5-4-3-1 Imaging Service Request Module .....	5-4
5-4-4 Requested Procedure Entity Module .....	5-4
5-4-4-1 Requested Procedure Module .....	5-4
5-4-5 Scheduled Procedure Step Entity Module .....	5-4
5-4-5-1 Scheduled Procedure Step Module .....	5-4
5-4-5-2 SOP Common Module .....	5-4

## REVISION HISTORY

REV	DATE	REASON FOR CHANGE
0	Nov. 24, 1995	Initial release to Direction Stock.
1	April, 1997	Basic Worklist Management Implementation for HIS/RISPatient/Study data retrieval parts of Section 2 and the complete Section 5

## LIST OF EFFECTIVE PAGES

PAGE NUMBER	REVISION NUMBER	PAGE NUMBER	REVISION NUMBER	PAGE NUMBER	REVISION NUMBER
Title Page	1				
Table of Contents i thru iv	1				
Revision History v thru vi	1				
Introduction 1-1 thru 1-6	1				
Conformance Statement 2-1 thru 2-6	1				
ADVANTX DLX3 Information Object Definition 3-1 thru 3-12	1				
Secondary Capture Implementation 4-1 thru 4-6	1				

**THIS PAGE LEFT INTENTIONALLY BLANK**



## SECTION 1 – INTRODUCTION

### 1–0 OVERVIEW

**Section 1, *Introduction***, provides general information about the content and scope of this document.

**Section 2, *Conformance Statement***, is the DICOM v3.0 Conformance Statement related to this product. Conformance Statements defines the subset of options selected from those offered by the DICOM v3.0 standard.

**Section 3, *DLX3 XRAY Angiographic Information Object Implementation*** defines the technical specifications required to interoperate with a DICOM v3.0 network interface. They define the technical details of the Information Object Definitions (IOD's) listed in the Conformance Statement. This section contains also the description of the private elements used in this implementation.


**Section 4, *Secondary Capture Image Information Object implementation***, defines the technical specifications required to interoperate with a DICOM v3.0 network interface. They define the technical details of the Information Object definition (IOD's) listed in the Conformance statement. This section contains also the description of the private elements used in this implementation.

**Section 5, *Basic Worklist Management Implementation***, defines the technical specifications required to interoperate with a DICOM v3.0 network interface. They define the technical details of the Information Object Definitions (IOD's) listed in the Conformance Statement.

### 1–1 OVERALL CONFORMANCE STATEMENT DOCUMENT STRUCTURE

The Documentation Structure of the ID/Net v3.0 Conformance Statements and their relationship with the DICOM v3.0 Conformance Statements is shown in Illustration 1–1.

ILLUSTRATION 1-1  
DOCUMENTATION STRUCTURE

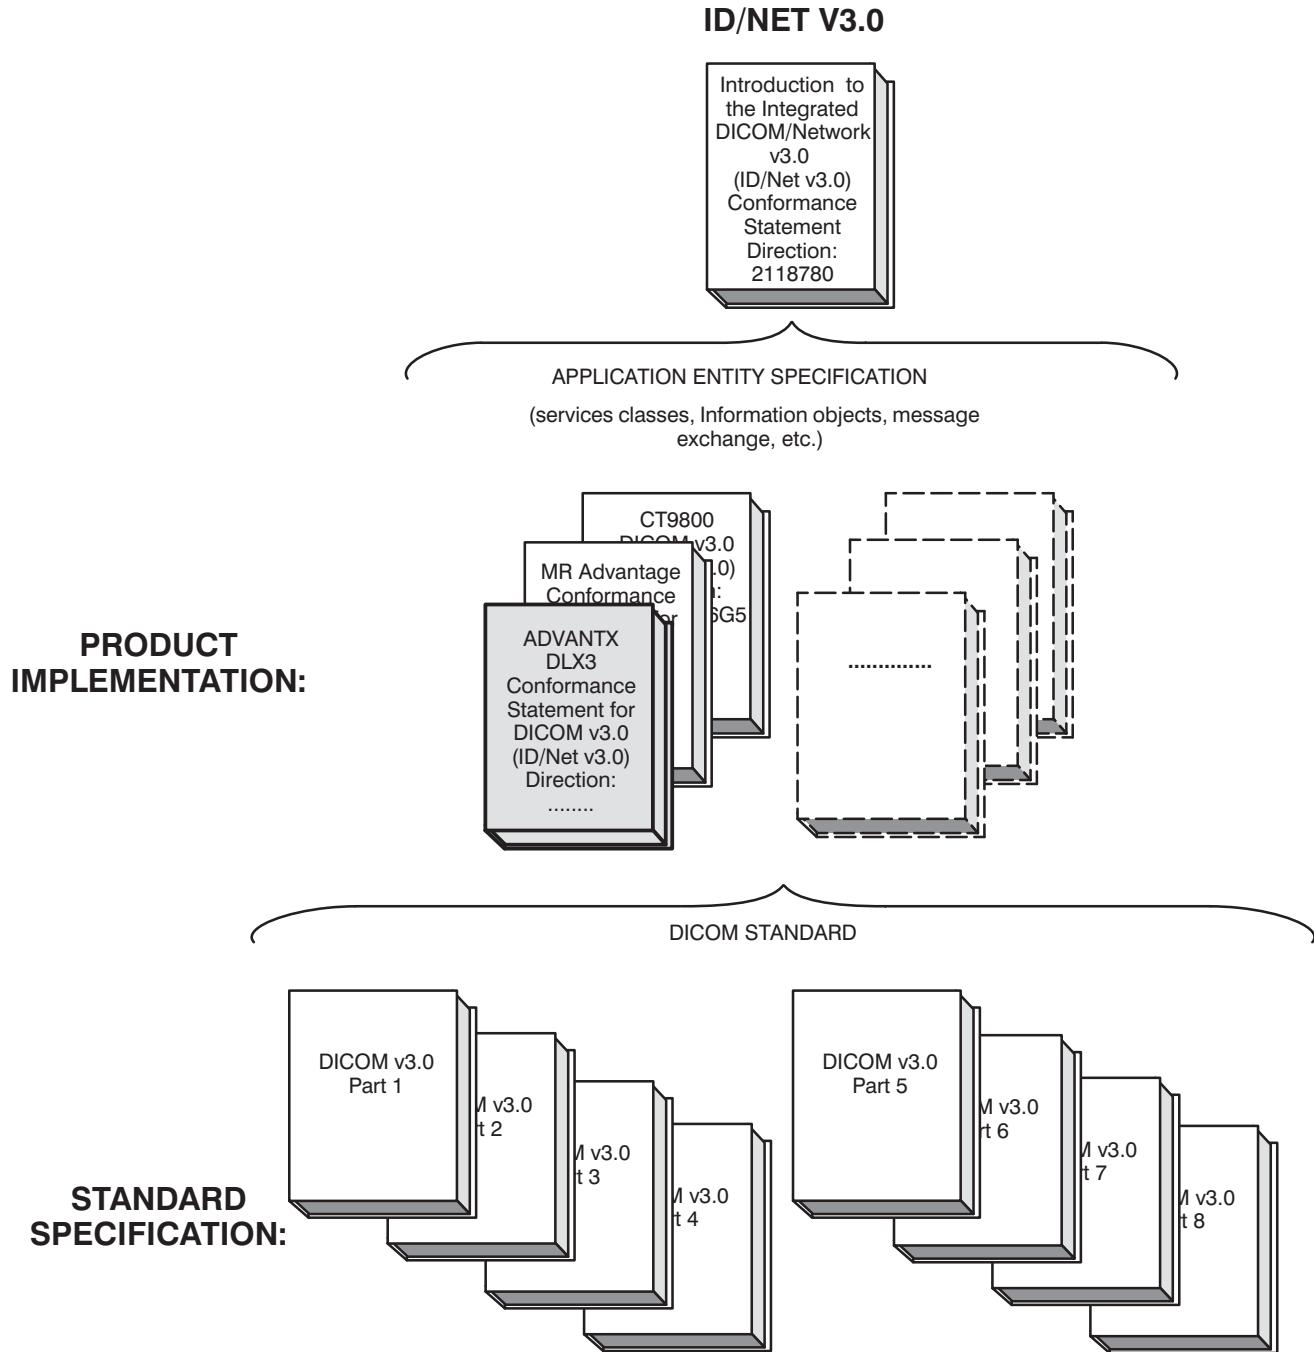

This document specifies the DICOM v3.0 implementation. It is entitled:

*ADVANTX DLX*

*Conformance Statement for DICOM v3.0 (ID/Net v3.0)*

*Direction .....# 2142506–100*

This Conformance Statement documents the DICOM v3.0 Conformance Statement and Technical Specification required to interoperate with the GEMS ID/Net v3.0 network interface. Introductory information, which is applicable to all GEMS ID/Net v3.0 Conformance Statements, is described in the document:

*Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0)*

*Conformance Statement*

*Direction: 2118780.*

This Introduction familiarizes the reader with DICOM terminology and general concepts. It should be read prior to reading the individual products' ID/Net v3.0 Conformance Statements.

The ID/Net v3.0 Conformance Statement, contained in this document, also specifies the Lower Layer communications which it supports (e.g., TCP/IP). However, the Technical Specifications are defined in the DICOM v3.0 Part 8 standard.

For more information including Network Architecture and basic DICOM concepts, please refer to the *Introduction*.

For the convenience of software developers, there is “collector” Direction available. By ordering the collector, the Introduction described above and all of the currently published ID/Net v3.0 Product Conformance Statements will be received. The collector Direction is:

*ID/Net v3.0 Conformance Statements*

*Direction: 2117016*

For more information regarding DICOM v3.0, copies of the Standard may be obtained by written request or phone by contacting:

NEMA Publication

2101 L Street, N.W., Suite 300

Washington, DC 20037 USA

Phone: (202) 457–8474

## 1–2

### INTENDED AUDIENCE

The reader of this document is concerned with software design and/or system integration issues. It is assumed that the reader of this document is familiar with the DICOM v3.0 Standards and with the terminology and concepts which are used in those Standards.

If readers are unfamiliar with DICOM v3.0 terminology they should first refer to the document listed below, then read the DICOM v3.0 Standard itself, prior to reading this Conformance Statement document.

*Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0)*

*Conformance Statement*

*Direction: 2118780*

### 1–3 SCOPE AND FIELD OF APPLICATION

It is the intent of this document, in conjunction with the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*, to provide an unambiguous specification for GEMS ID/Net v3.0 implementations. This specification, called a Conformance Statement, includes a DICOM v3.0 Conformance Statement and is necessary to ensure proper processing and interpretation of GEMS medical image data exchanged using DICOM v3.0. The GEMS ID/Net v3.0 Conformance Statements are available to the public.

The reader of this Conformance Statement should be aware that different GEMS devices are capable of using different Information Object Definitions. For example, a GEMS CT Scanner may send images using the CT Information Object, MR Information Object, Secondary Capture Object, etc.

Included in this Conformance Statement are the Module Definitions which define all data elements used by this GEMS ID/Net v3.0 implementation. If the user encounters unspecified private data elements while parsing a GEMS Data Set, the user is well advised to ignore those data elements (per the DICOM v3.0 standard). Unspecified private data element information is subject to change without notice. If, however, the device is acting as a "full fidelity storage device", it should retain and retransmit all of the private data elements which are sent by GEMS devices.

### 1–4 IMPORTANT REMARKS

The use of these Conformance Statements, in conjunction with the DICOM v3.0 Standards, is intended to facilitate communication with GE imaging equipment. However, **by itself, it is not sufficient to ensure that inter-operation will be successful**. The **user (or user's agent)** needs to proceed with caution and address at least four issues:

- **Integration** – The integration of any device into an overall system of interconnected devices goes beyond the scope of standards (DICOM v3.0), and of this introduction and associated Conformance Statements when interoperability with non-GE equipment is desired. The responsibility to analyze the applications requirements and to design a solution that integrates GE imaging equipment with non-GE systems is the **user's** responsibility and should not be underestimated. The **user** is strongly advised to ensure that such an integration analysis is correctly performed.
- **Validation** – Testing the complete range of possible interactions between any GE device and non-GE devices, before the connection is declared operational, should not be overlooked. Therefore, the **user** should ensure that any non-GE provider accepts full responsibility for all validation required for their connection with GE devices. This includes the accuracy of the image data once it has crossed the interface between the GE imaging equipment and the non-GE device and the stability of the image data for the intended applications. Such a validation is required before any clinical use (diagnosis and/or treatment) is performed. It applies when images acquired on GE imaging equipment are processed/displayed on a non-GE device, as well as when images acquired on non-GE equipment is processed/displayed on a GE console or workstation.

- **Future Evolution** – GE understands that the DICOM Standard will evolve to meet the user’s growing requirements. GE is actively involved in the development of the DICOM v3.0 Standard. DICOM v3.0 will incorporate new features and technologies and GE may follow the evolution of the Standard. ID/Net v3.0 is based on DICOM v3.0 as specified in each ID/Net DICOM Conformance Statement. Evolution of the Standard may require changes to devices which have implemented DICOM v3.0. **In addition, GE reserves the right to discontinue or make changes to the support of communications features (on its products) reflected on by these ID/Net DICOM Conformance Statements.** The user should ensure that any non-GE provider, which connects with GE devices, also plans for the future evolution of the DICOM Standard. Failure to do so will likely result in the loss of function and/or connectivity as the DICOM Standard changes and GE Products are enhanced to support these changes.
- **To be kept informed of the evolution of the implementation described in this document, the User should register on the GE Internet Server, accessible via anonymous ftp, by entering his e–mail address (GE Internet Server Address: ftp.med.ge.com, 192.88.230.11)**
- **Interaction** – It is the sole responsibility of the **non-GE provider** to ensure that communication with the interfaced equipment does not cause degradation of GE imaging equipment performance and/or function.

**1–5****REFERENCES**

A list of references which is applicable to all ID/Net v3.0 Conformance Statements is included in the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780.*

The information object implementation refers to the X-Ray Radiofluoroscopic Image Object Definition (DICOM v3.0 Standard Supplement 6) to Part 3 (Information Object Definition)

**1–6****DEFINITIONS**

A set of definitions which is applicable to all ID/Net v3.0 Conformance Statements is included in the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780.*

**1–7****SYMBOLS AND ABBREVIATIONS**

A list of symbols and abbreviations which is applicable to all ID/Net v3.0 Conformance Statements is included in the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780.*

**THIS PAGE LEFT INTENTIONALLY BLANK**

## SECTION 2 – CONFORMANCE STATEMENT

### 2-0 INTRODUCTION

This conformance statement (CS) specifies the GE Advantx DLX compliance to DICOM v3.0. It details the DICOM Service Classes and roles which are supported by this product.

Advantx DLX is an Integrated Digital Vascular Imaging System for both Angiography and Cardiac applications. It uses DICOM services to export images to remote workstations


Note that the format of this section strictly follows the format of DICOM Standard Part 2 (Conformance) Annex A. Please refer to that part of the standard while reading this section.

### 2-1 IMPLEMENTATION MODEL

#### 2-1-1 Application Data Flow Diagram

The Basic and Specific Application models for this device are shown in Ill. 2-1 .

ILLUSTRATION 2-1  
SPECIFIC AE APPLICATION MODEL

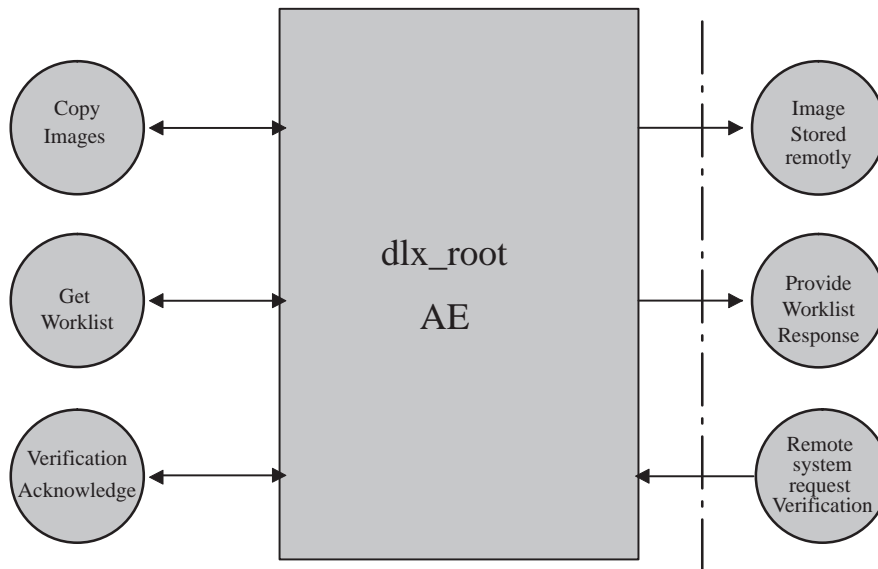

The dlx\_root Application Entity (AE) is an application which handles DICOM protocol communication. dlx\_root AE is automatically brought up when the Digital Angiographic system (DLX) is powered on.

All remote DICOM's AE must be manually configured on the DLX, usually at the software installation time, by a GE field engineer.

There are 2 local real world activities: Copy Image (CI) and Get Worklist (GW) which can cause the dlx\_root AE to initiate a DICOM association.

CI consists of an operator selecting one or several images to be sent on one or several Remote System(s). Selection of Images is done from the Operator console screens (known as BROWSER and VIEWER); selection of Remote Systems and visualisation of the status of the transfer is done on a specific menu (known as TRANSFER menu) . Remote Workstation can be any DICOM compliant WorkStation.

GW consists of an operator request for the transfer of a list of Patient/Exam entries from a predefined remote HIS/RIS system. There is no query key set for subselection of items. The current implementation asks for all data prepared for transfer to DLX. The remote workstation can be any DICOM compliant HIS/RIS system supporting XA modality.

**2–1–2 Functional Definition of AE’s**

The dlx\_root Application Entity supports the following two SCU functions (one at a time):

1. Copy Images:

- Access to patient demographics and Pixel Data in the local database.
- Build a DICOM format data set.
- Initiate a DICOM association to send the image(s).

2. Get Worklist:

- Build a DICOM formatted basic worklist management data request.
- Initiate a DICOM association to send the request.
- Wait for worklist response(s).
- Access the local database to add new patient/exam demographic data.
- Close the open Association.

The dlx\_root Application Entity also serves a default SCP function, the verification (Echo) Service Class request, independently from the other SCU functions.

**2–1–3 Sequencing of Real–World Activities**

Not Applicable

**2–2 AE SPECIFICATIONS**

**2–2–1 AE Specification**

This Application Entity provides Standard Conformance to the following DICOM V3.0 SOP Classes as an SCU:

SOP Class Name	SOP Class UID
X–Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7

X–Ray Angiographic Image Storage is implemented as a Standard Extended SOP Class. It contains type 3 private Data Elements.

Standard conformance as an SCP is not applicable for this Application Entity.

This Application Entity provides Standard Conformance to the following DICOM V3.0 SOP Class as an SCP :

SOP Class Name	SOP Class UID
Verification Service Class	1.2.840.10008.1.1



**2–2–1–1 Association Establishment Policies**

**2–2–1–1–1 General**

The DICOM Application Context Name (ACN), which is always proposed, is:

<b>Application Context Name</b>	<b>1.2.840.10008.3.1.1.1</b>
---------------------------------	------------------------------

The Maximum Length PDU negotiation is included in all association establishment requests.

The maximum length PDU for an association initiated by the dlx\_root AE is:

<b>Maximum Length PDU</b>	<b>16 Kbytes</b>
---------------------------	------------------

The SOP class Extended Negotiation is not supported.

The maximum number of Presentation Contexts Items that will be proposed is 2.

The user info items sent by this product are:

- Maximum PDU Length
- Implementation UID

**Note:** Max PDU length can be configured at installation time.

**2–2–1–1–2 Number of Associations**

The dlx\_root AE will Initiate only one DICOM association to perform an image storage or a Worklist transfer as an SCU to a remote host.

The dlx\_root AE will not support multiple SCU associations simultaneously. The verification SCP association can be open simultaneously to another SCU association.

**2–2–1–1–3 Asynchronous Nature**

Asynchronous mode is not supported. All operations will be performed synchronously.

**2–2–1–1–4 Implementation Identifying Information**

The Implementation UID for this ID/Net v3.0 Implementation is:

<b>AdvantX DLX Implementation UID</b>	<b>1.2.840.113619.6.33</b>
---------------------------------------	----------------------------

**2–2–1–2 Association Initiation Policy**

dlx\_root AE attempts to initiate a new association for each image it attempts to transfer. This association corresponds to one Real–World Activity: Copy Image(CI) or Get Worklist (GW).

**2–2–1–2–1 Real–World Activity ”Copy Image”**

**2–2–1–2–1–1 Associated Real–World Activity**

The operator selects a destination by selecting an Host in the ‘TRANSFER’ menu (by default the last selected host is active).

Then he selects Image(s) to be sent by selection in both BROWSER (at patient level), or VIEWER (at sequence or photo level).

This operation will cause

- the dlx\_root AE to initiate a DICOM association.
- the dlx\_root AE to emit a C–ECHO command to check if the remote AE is available.
- the DLX to build a DICOM image from its compressed raw data
- the dlx\_root AE to initiate a DICOM association, select the appropriate Abstract and Transfer syntax from those accepted by the remote AE
- the dlx\_root AE to emit C–STORE command to send the image.

**2–2–1–2–1–2 Proposed Presentation Contexts**

Presentation Context Table – Proposed					
Abstract Syntax		Transfer Syntax		Role	Expanded Negotiation
Name	UID	Name List	UID List		
XRAY Angio Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

**2–2–1–2–1–2–1SOP Specific Conformance Statement for Image Storage SOP Class**

This implementation performs a single C–STORE operation over an association.

If the AE doesn’t receive a C–ECHO confirmation, this implementation will terminate the association. The transfer is considered as failed, no association for C–STORE will be attempted.

Upon receiving a C–ECHO confirmation containing an Error, Refused or Warning status, this implementation will consider the result as OK. This is because the only purpose of the C–ECHO is to check that the remote AE responds, whatever is the C–ECHO status. This implementation doesn’t require that remote AE implements Verification SOP class as a SCP.

Upon receiving a C–STORE confirmation containing an Error or a Refused status, this implementation will terminate the association. The current C–STORE is considered as failed.

Upon receiving a C–STORE confirmation containing a Warning Status, this implementation will treat it as an Error or Refused response.

Each C–STORE operation supports an “ Association Timer ”. This timer starts when the association request is sent and stops when the association is established. This timer is set to 60 seconds.

Each C–STORE operation supports an “ Operation Inactivity Timer ”. This timer starts once a C–STORE request has been issued and stops once a C–STORE confirmation has been received. This Timer is set to 60 minutes.

If any of the 2 timers expires, the connection is closed and the operation is considered as failed.

**2–2–1–2–2 Real–World Activity ”Get Worklist”**

**2–2–1–2–2–1 Associated Real–World Activity**

The Worklist option has to be enabled by the system installation procedure.

The operator selects a destination host through a service menu.

The worklist transfer can be initiated from the Patient Viewer Dialogue by pressing the “Worklist” soft key.

This operation will cause:

- the dlx\_root AE to initiate a DICOM association.
- the dlx\_root AE to emit a C–ECHO request to check if the remote AE is available. Finally the association is closed.
- the DLX to build a Basic Worklist C–FIND Request.
- the dlx\_root AE to initiate a DICOM association, select the appropriate Abstract and Transfer Syntax from those accepted by the remote AE.
- the dlx\_root AE to emit the C–FIND Request.
- the dlx\_root AE to receive C–FIND (Worklist) Response(s).
- the DLX to add new entry items to the local database if they are not existing yet.
- the dlx\_root AE to close the association.

**2–2–1–2–2–2 Proposed Presentation Contexts**

Abstract Syntax		Transfer Syntax		Role	Expanded Negotiation
Name	UID	Name	UID		
Modality		Implicit VR		SCU	none
Worklist	1.2.840.10008.5.1.4.31	Little	1.2.840.10008.1.2		
Information		Endian			
Model – FIND					

**2–2–1–2–2–2–1 SOP Specific Conformance Statement for Image Storage SOP Class**

This implementation performs a single C–FIND operation over one association.

If the AE does not receive a C–ECHO confirmation, this implementation will terminate the association. The Worklist request is considered as failed.

Upon receiving a C–ECHO confirmation containing an Error, Refused or Warning status, this implementation will consider the result OK. This is because the only purpose of the C–ECHO is to check that the remote AE responds.

Each C–ECHO and C–FIND operation supports an “Association Timer”. This timer starts when the association request is sent and the stops when the association is established. This timer is set to 30 seconds.

The C-ECHO operation supports an “Operation Inactivity Timer”. This timer starts when the C-ECHO request is sent and it stops when the C-ECHO response is received. This timer is also set to 30 seconds.

Upon receiving a C-FIND response containing an error status this implementation will terminate the association issuing a close request. The current C-FIND is considered as failed.

Each C-FIND operation supports an “Operation Inactivity Timer”. This timer starts when the C-FIND request is sent and it stops when the C-FIND final response received. This timer is set to 60 seconds.

If any of the timers expires, the connection is closed and the operation is considered as failed.

Badly formatted C-FIND response(s) from the SCP will result in the initiation of a C-FIND cancel request. In the dlx\_root AE, the C-FIND cancel operation is not implemented as an additional operator choice.

On completion of operation the dlx\_root AE places the status (flag) of the final Worklist update operation on DLX into the Abort flag of the close association request. That way the Worklist provider can get a final success feed back of the complete HIS/RIS data transfer operation. This flag setting doesn’t change the basic DICOM association management functionality.

**2-2-1-3 Association Acceptance Policy**

The dlx\_root AE provides only DICOM Verification Service Class.

**2-2-1-3-1 Real-World Activity ”Verification acknowledge”**

DLX echoes to a Verification request from any DICOM node. This function is transparent to the user (no user interface, no message logged on screen).

**2-2-1-3-1-1 Associated Real-World Activity**

**2-2-1-3-1-2 Accepted Presentation Contexts**

Presentation Context Table – Accepted					
Abstract Syntax		Transfer Syntax		Role	Expanded Negotiation
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

**2-2-1-3-1-2-1 SOP Specific Conformance Statement for Verification SOP Class**

The dlx\_root AE provides standard conformance to the DICOM Verification Service Class.

**2–3 COMMUNICATION PROFILES****2–3–1 Supported Communication Stacks (parts 8,9)**

DICOM Upper Layer (Part 8) is supported using TCP/IP.

**2–3–2 TCP/IP Stack**

The TCP/IP stack is inherited from a UNIX Operating System.

**2–3–2–1 API**

Not applicable to this product.

**2–3–2–2 Physical Media Support**

Ethernet v2.0, IEEE 802.3.

**2–3–3 Point-to-Point Stack**

A 50–pin ACR–NEMA connection is not applicable to this product.

**2–4 EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS**

Refer to Section 3 for the description of AdvantX DLX Private DICOM Data Dictionary

Refer to Section 4 for the description of Secondary capture Private DICOM Data Dictionary

**2–5 CONFIGURATION****2–5–1 AE Title/Presentation Address Mapping**

The Local AE Title is configurable. This must be configured by a GEMS Field Service Engineer during an installation.

**2–5–2 Configurable Parameters**

The following fields are configurable for this AE (local):

- Local AE Title
- Local IP Address

The following fields are configurable for every remote DICOM AE:

- Remote AE Title
- Responding TCP/IP Port
- Remote IP Address

**Note:** All configuration must be performed by a GE Field Engineer.

**2–6 SUPPORT OF EXTENDED CHARACTER SETS**

This implementation supports the following extended character set:  
ISO–IR–100



## SECTION 3 XA INFORMATION OBJECT IMPLEMENTATION

### 3-0 INTRODUCTION


This section specifies the use of the DICOM v3.0 XRAY Angiographic Image IOD to represent the information included in XRAY Angiographic images produced by this implementation. Corresponding attributes are conveyed using the module construct.

### 3-1 XA IMAGE IOD IMPLEMENTATION

This section defines the implementation of XA image information object. It refers to the DICOM V3.0 Standard, Supplement 4 (Oct 21, 1995) to Part 3 (Information Object definition).

### 3-2 XA IMAGE IOD ENTITY-RELATIONSHIP MODEL

**Illustration 3-1**  
**XRAY Angiographic Image Entity Relationship Diagram**

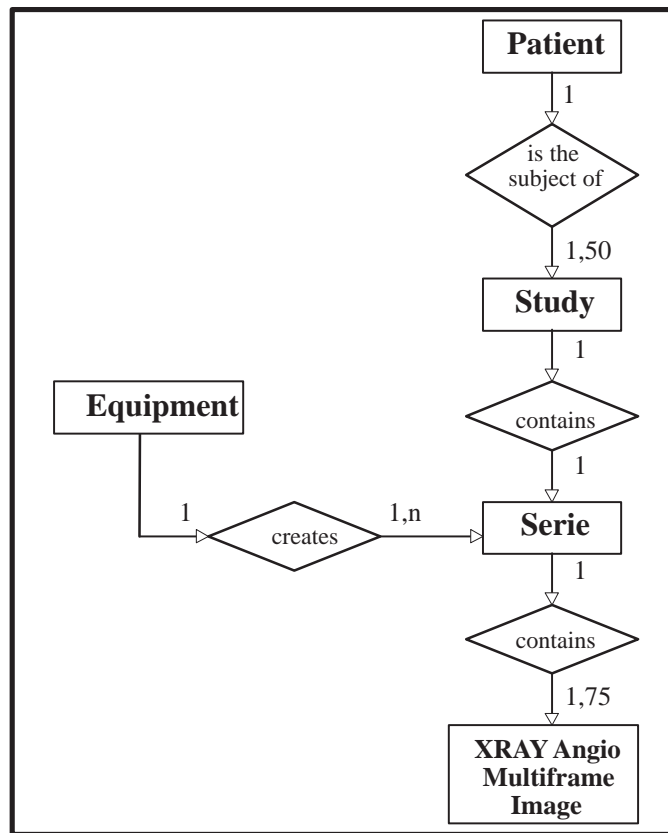

The Entity–Relationship diagram for the XRAY Angiographic Image interoperability schema is shown in Illustartion 3–1. In this figure, the following diagrammatic convention is established to represent the information organisation :

- each entiy is represented by a rectangular box
- each relationship is represented by a diamond shaped box.
- the fact that a relationship exists between two enties is depicted by lines connecting the corresponding entity boxes to the relationships boxes.

The relationships are fully defined with the maximum number of possible entities in the relationship shown.

**3–2–1 Entities Description**

Refer to DICOM Standard Supplement 4 (Oct 21, 1995) to Part 3 (Information Object Definitions) for a description of the entities contained within this Information object.

**3–2–2 DLX Mapping of DICOM entities**

DICOM entities map to the DLX entities in respect to the following :

DICOM	DLX
Patient Entity	Patient Entity
Study Entity	Examination Entity
Serie Entity	no match, there is a one to one relationship between DICOM Study and Serie
Multiframe Image Entity	Sequence Entity
Frame	Image

**3–3 XA IMAGE IOD MODULE TABLE**

Within an entity of the DICOM v3.0 XRAY Angio Image Information Object Definition, attributes are grouped into related set of attributes. A set of related attributes is termed a module. A module acilitates the understanding of the semantics concerning the attributes and how the attributes are related with each other. A module grouping does not infer any encoding of information into datasets.

Table 2 identifies the defined modules within the entities which comprise the DICOM v3.0 XRAY Angio Image Information object Definition. Modules are identified by Module Name.

See DICOM v3.0 Part 3 for a complete definition of the entities, modules, and attributes.



**Table 2**  
**XRAY Angiographic Image Information Object Definition (IOD) Module Table**

IE	Module Name	Reference
Patient	Patient	3.4.1.1
Study	General Study	3.4.2.1
	Patient Study	3.4.2.2
Series	General Series	3.4.3.1
Equipment	General Equipment	3.4.4.1
Image	General Image	3.4.5.1
	Image Pixel	3.4.5.2
	Cine	3.4.5.3
	Multi-Frame	3.4.5.4
	Frame Pointers	3.4.5.5
	Mask	3.4.5.6
	Display Shutter	3.4.5.7
	Device	3.4.5.8
	X-Ray Image	3.4.5.9
	X-Ray Acquisition	3.4.5.10
	X-Ray Collimator	3.4.5.11
	X-Ray Table	3.4.5.12
	XA Positioner	3.4.5.13
	Curve	3.4.5.14
	SOP Common	3.4.5.15

**3-4 INFORMATION MODULE DEFINITIONS**

Please refer to DICOM v3.0 Standard Part 3 (Information Object Definition) for a description of each of the entities and modules contained within the XRAY Angiographic Information Object.

Modules contain also **type 3 Private elements**.

**3-4-1 Patient Entity Module**

**3-4-1-1 Patient Module**

Attribute Name	Element Tag	TP	Notes
Patient's Name	0010, 0010	2	
Patient ID	0010, 0020	2	
Patient's Birth Date	0010, 0030	2	No value, Zero length
Patient's Sex	0010, 0040	2	
Patient DOB	0011, xx01	3	Patient Date of Birth in free form.

**3-4-2 Study Entity Module****3-4-2-1 General Study**

Attribute Name	Element Tag	TP	Notes
Study Instance UID	0020, 000D	1	
Study Date	0008, 0020	2	
Study Time	0008, 0030	2	
Referring Physicians' Name	0008, 0090	2	
Study ID	0020, 0010	2	
Accession number	0008, 0050	2	No value, Zero length
Study Description	0008, 1030	3	

**3-4-2-2 Patient Study**

Attribute Name	Element Tag	TP	Notes
Patient's Size	0010, 1020	3	
Patient's Weight	0010, 1030	3	
Additional Patient's History	0010, 21B0	3	
Patient address	0010, 1040	3	
Patient telephone	0010, 2154	3	

**3-4-3 Series Entity Module****3-4-3-1 General Series**

Attribute Name	Element Tag	TP	Notes
Modality	0008, 0060	1	XA
Series Instance UID	0020, 000E	1	
Series Number	0020, 0011	2	1
Series Date	0008, 0021	3	
Series Time	0008, 0031	3	
Performing Physician's Name	0008, 1050	3	
Series Description	0008, 103E	3	
Operators' Name	0008, 1070	3	

**3-4-4 Equipment Entity Module****3-4-4-1 General Equipment**

Attribute Name	Element Tag	TP	Notes
Manufacturer	0008, 0070	3	GE MEDICAL SYSTEMS
Institution Name	0008, 0080	3	
Manufacturer Model Name	0008, 1090	3	DLX
Software versions	0018, 1020	3	

**3-4-5 Image Entity Module****3-4-5-1 General Image**

Attribute Name	Element Tag	TP	Notes
Image Number	0020,0013	2	Image number in the serie
Image Date	0008,0023	2C	
Image Time	0008,0033	2C	
Image Type	0008,0008	3	ORIGINAL\PRIMARY\ either SINGLE PLANE, BIPLANE A or BIPLANE B
Acquisition Date	0008,0022	3	
Acquisition Time	0008,0032	3	
Patient Orientation	0020,0020	2	No value, Zero length
Image comments	0020,4000	3	
Referenced Image Sequence	0008, 1140	3	In case of DLX biplane acquisition, used to identify the related plane Image (LATeral if FRonTal or FRonTal if LATeral)
>Referenced SOP Class UID	0008, 1150	1C	1.2.840.10008.5.1.4.1.1.12.1
>Referenced SOP Instance UID	0008, 1155	1C	
Lossy Image Compression	0028, 2110	3	0
Side_mark	0019, xx1D	3	represents patient orientation as 2 characters located on the left and right side of the displayed frame. Encoding is the following : 0 : not defined 1, 4, 6 : Left of the patient is on the left side of the frame 2, 3, 5 : Right of the patient is on the left side of the frame

**3-4-5-2 Image Pixel**

Attribute Name	Element Tag	TP	Notes
Samples per Pixel	0028, 0002	1	1
Photometric Interpretation	0028, 0004	1	MONOCHROME 2
Rows	0028, 0010	1	512 or 1024
Columns	0028, 0011	1	512 or 1024
Bits Allocated	0028, 0100	1	8 or 16
Bits Stored	0028, 0101	1	8 or 10
High Bit	0028, 0102	1	7 or 9
Pixel Representation	0028, 0103	1	0
Pixel Data	7FE0, 0010	1	

**3-4-5-3 Cine**

Attribute Name	Element Tag	TP	Notes
Frame Time Vector	0018, 1065	1C	
Start Trim	0008, 2142	1	
Stop Trim	0008, 2143	1	
Recommended Display Frame Rate	0008, 2144	1	
Frame Delay	0018, 1066	1	
Cine Rate	0018, 0040	1	

**3-4-5-4 Multi-Frame**

Attribute Name	Element Tag	TP	Notes
Number of Frames	0028, 0008	1	
Frame Increment pointer	0028, 0009	1	0018, 1065

**3-4-5-5 Frame Pointers**

Attribute Name	Element Tag	TP	Notes
Representative Frame Num- ber	0028, 6010	3	Initialized as the frame number located at the 1/3rd of the multiframe image.
Cur_spatial_filter_strength	0019, xx17	3	
Zoom_factor	0019, xx18	3	1, 2 or 4
X_zoom	0019, xx19	3	coordinate of the center of the zoomed area
Y_zoom	0019, xx1A	3	coordinate of the center of the zoomed area
Text_annotation	70nn, xx04	3	There could be up to 5 annoation per images
Box	70nn, xx05	3	Coordinates of the lower left corner of the first character of the annotation (x, y)
Arrow end	70nn, xx07	3	Coordinates of extrens of the arrow (x, y), the arrow always starts from the annotation text. Arrows is always a staight line. (0,0) value means 'no arrow' is attached to the annotation.

**3-4-5-6 Mask**

Attribute Name	Element Tag	TP	Notes
Mask Subtraction Sequence	0028, 6100	1	
>Mask Operation	0028, 6101	1C	NONE or AVG_SUB
>Applicable Frame Range	0028, 6102	3	
>Mask Frame Numbers	0028, 6110	1C	
>Mask Sub-pixel shift	0028, 6114	3	
Percentage_landscape	0019, xx1E	3	Percentage of mask applied

**3-4-5-7 Display Shutter**

Attribute Name	Element Tag	TP	Notes
Shutter Shape	0018, 1600	1	CIRCULAR or RECTANGULAR. Combined Rectangular and Circular could exist and is represented by both RECTANGULAR/CIRCULAR attributes.
Display Shutter Left Vertical Edge	0018, 1602	1C	
Display Shutter Right Vertical Edge	0018, 1604	1C	
Display Shutter Upper Horizontal Edge	0018, 1606	1C	
Display Shutter Lower Horizontal Edge	0018, 1608	1C	
Center of Circular Display Shutter	0018, 1610	1C	
Radius of Circular Display Shutter	0018, 1612	1C	

**3-4-5-8 Device**

Attribute Name	Element Tag	TP	Notes
Device Sequence	0050, 0010	3	
>Code Value	0008, 0100	1C	BALL or CATHETER
>Coding Scheme Designator	0008, 0102	1C	99DEV
>Device Diameter	0050, 0016	3	
>Device Diameter Units	0050, 0017	2C	
Stenos_calibr_ratio;	0015, xx01	3	Calibration ratio for Stenosis Quantification, expressed for a 1024 pixel matrix.
Stenos_magnification;	0015, xx02	3	Calibration ratio for Length measurement
Cardiac_calibr_ratio;	0015, xx03	3	Calibration ratio for VG quantification

**3-4-5-9 X-Ray Image**

Attribute Name	Element Tag	TP	Notes
Frame Increment pointer	0028, 0009	1C	
Lossy Image Compression	0028,2110	1C	0
Image Type	0008, 0008	1	ORIGINAL\PRIMARY\ either SINGLE PLANE, BIPLANE A or BIPLANE B
Pixel Intensity Relationship	0028, 1040	1	value : LIN, or DISP. In DISP mode, only spatial measurements are available.
Samples per Pixel	0028,0002	1	1
Photometric interpretation	0028,0004	1	MONOCHROME1\MONOCHROME 2
Bits allocated	0028, 0100	1	8 or 16
Bits stored	0028, 0101	1	8 or 10
High Bit	0028, 0102	1	7 or 9
Pixel Representation	0028, 0103	1	0
Reference Image Sequence	0008, 1140	3	Used to identify the related plane Image in case of Biplane acquisition (LATeral if FRonTal or FRonTal if LATeral)
>Reference SOP class UID	0008, 1150	1C	
>Reference SOP instance UID	0008, 1155	1C	
R Wave Pointer	0028, 6040	3	
Scan Options	0018, 0022	3	EKG or STEP, or CHASE, or ROTA

**3-4-5-10 X-Ray Acquisition**

Attribute Name	Element Tag	TP	Notes
KVP	0018, 0060	3	
Field of view Shape	0018, 1147	3	ROUND
Field of View Dimension	0018, 1149	3	
Grid	0018, 1166	3	IN
Radiation Mode	0018, 115A	3	PULSED
Radiation Setting	0018, 1155	1	GR
X-ray Tube Current	0018, 1151	3	
Intensifier Size	0018,1162	3	
Adx_procedure_name	0019, xx07	3	free text information
Adx_exam_name	0019, xx08	3	free text information
Adx_patient_size	0019, ,xx09	3	LOW, MEDIUM, ADULT
Adx_injector_delay	0019, xx10	3	delay in start of injection in 1/10th of seconds
Adx_auto_inject	0019, xx11	3	1 if autoinjection, 0 if not
Adx_acq_mode	0019, xx14	3	0,1 for vascular 2..7 for cardiac 8..13 for DSA stepping 14..19, 26 for Bolus Chasing 20..25 for HSS acquisition
Adx_camera_rotation_enable	0019, xx15	3	0..3 rotation disabled 4..7 rotation enabled

Attribute Name	Element Tag	TP	Notes
Adx_reverse_sweep	0019, xx16	3	0,4 no reverse sweep 1, 5 vertical reverse sweep 2, 6 horizontal reverse sweep 3, 7 Horizontal & Vertical sweep
Adx_focus	0019, xx1B	3	focus on frontal plane
Adx_dose	0019, xx1C	3	0, 1, 2, 3 for dose A, B, C, D
Adx_exposure_duration	0019, xx1F	3	in ms.
Acq_Record View	0019, 000A	3	1 Frontal, 2 Lateral 3 Biplane

**3-4-5-11 X-Ray Collimator**

Attribute Name	Element Tag	TP	Notes
Collimator shape	0018,1700	1	value : CIRCULAR
Center of circular collimator	0018,1710	1C	
Radius of circular Collimator	0018,1712	1C	

**3-4-5-12 X-Ray table**

Attribute Name	Element Tag	TP	Notes
Table Motion	0018, 1134	2	DYNAMIC or STATIC
Table Vertical Increment	0018, 1135	2C	0
Table Longitudinal Increment	0018, 1137	2C	
Table Lateral Increment	0018, 1136	2C	0

**3-4-5-13 XA Positioner**

Attribute Name	Element Tag	TP	Notes
Distance Source to Patient	0018, 1111	3	
Distance Source to detector	0018, 1110	3	
Estimated Radiographic Magnification factor	0018, 1114	3	
Positioner Motion	0018, 1500	2C	STATIC or DYNAMIC
Positioner Primary Angle	0018, 1510	2	
Positioner Secondary Angle	0018, 1511	2	
Positioner Primary Angle Increment	0018, 1520	2C	
Positioner Secondary Angle Increment	0018, 1521	2C	
Angle_value_1	0019, xx01	3	Positioner angle for L arm in degrees
Angle_value_2	0019, xx02	3	Positioner angle for P arm in degrees
Angle_value_3	0019, xx03	3	Positioner angle for C arm in degrees
Angle_label_1	0019, xx04	3	L
Angle_label_2	0019, xx05	3	CAU, CRA
Angle_label_3	0019, xx06	3	LAO, RAO

**3-4-5-14 Curve**

Attribute Name	Element Tag	TP	Notes
Curve Dimensions	50xx, 0005	1	
Number of points	50xx, 0010	1	
Type of Data	50xx, 0020	1	ROI or PHYSIO
Data Value Representation	50xx, 0103	1	0
Curve Data	50xx, 3000	1	
Curve Description	50xx, 0022	3	only if Type of Data (50xx, 0020) = ROI, then 1 for diastolic 0 for systolic

Curves can be either Cardiac Contours (1 diastolic and 1 systolic per multiframe image), or a physiological curve (e.g. EKG). For a Multiframe Image, there could be 2 Cardiac contour and 2 physiological curves.

**3-4-5-15 SOP Common**

Attribute Name	Element Tag	TP	Notes
SOP Class UID	0008, 0016	1	1.2.840.10008.5.1.4.1.1.12.1
SOP Instance UID	0008, 0018	1	
Specific Character	0008, 0005	1C	ISO-IR-100



PRIVATE DATA DICTIONARY

Attribute Name	Data Element Tag	VR	VM
<b>Private Creator PATIENT_01</b>	<b>0011,00xx</b>	<b>LO</b>	<b>1</b>
Patient DOB	0011, xx01	LT	1
<b>Private Creator EXAM_01</b>	<b>0015,00xx</b>	<b>LO</b>	<b>1</b>
Stenos_calibr_ratio;	0015, xx01	DS	1
Stenos_magnification;	0015, xx02	DS	1
Cardiac_calibr_ratio;	0015, xx03	DS	1
<b>Private Creator SERIE_01</b>	<b>0019,00xx</b>	<b>LO</b>	<b>1</b>
Angle_value_1	0019, xx01	DS	1
Angle_value_2	0019, xx02	DS	1
Angle_value_3	0019, xx03	DS	1
Angle_label_1	0019, xx04	CS	1
Angle_label_2	0019, xx05	CS	1
Angle_label_3	0019, xx06	CS	1
Adx_procedure_name	0019, xx07	ST	1
Adx_exam_name	0019, xx08	ST	1
Adx_patient_size	0019, xx09	SH	1
Acq_record view	0019, 000A	IS	1
Adx_injector_delay	0019, xx10	DS	1
Adx_auto_inject	0019, xx11	CS	1
Adx_acq_mod	0019, xx14	IS	1
Adx_camera_rotation_enable	0019, xx15	CS	1
Adx_reverse_sweep	0019, xx16	CS	1
Cur_spatial_filter_strength	0019, xx17	IS	1
Zoom_factor	0019, xx18	IS	1
X_zoom	0019, xx19	IS	1
Y_zoom	0019, xx1A	IS	1
Adx_focus	0019, xx1B	DS	1
Adx_dose	0019, xx1C	CS	1
Side_mark	0019, xx1D	IS	1
Percentage_landscape	0019, xx1E	IS	1
Adx_exposure_duration	0019, xx1F	DS	1
<b>Private Creator ANNOT_01</b>	<b>70nn,00xx</b>	<b>LO</b>	<b>1</b>
Text_annotation	70nn, xx04	ST	1
Box	70nn, xx05	IS	2
Arrow end	70nn, xx07	IS	2

Attribute Name	Data Element Tag	Value
Private Creator PATIENT_01	0011,00xx	DLX_PATNT_01
Private Creator EXAM_01	0015,00xx	DLX_EXAMS_01
Private Creator SERIE_01	0019,00xx	DLX_SERIE_01
Private Creator ANNOT_01	70nn,00xx	DLX_ANNOT_01

**THIS PAGE LEFT INTENTIONALLY BLANK**

## **SECTION 4 – SECONDARY CAPTURE IMPLEMENTATION**

### **4-0 INTRODUCTION**


This section specifies the use of the DICOM v3.0 Secondary Capture Image IOD to represent the information included in Secondary Capture images produced by this implementation. Corresponding attributes are conveyed using the module construct.

### **4-1 SC IMAGE IOD IMPLEMENTATION**

This section defines the implementation of SC image information object. It refers to the DICOM V3.0 Standard, Part 3 (Information Object definition).

### **4-2 SC IMAGE IOD ENTITY-RELATIONSHIP MODEL**

**Illustration 4-1**  
**SC Image Entity Relationship Diagram**

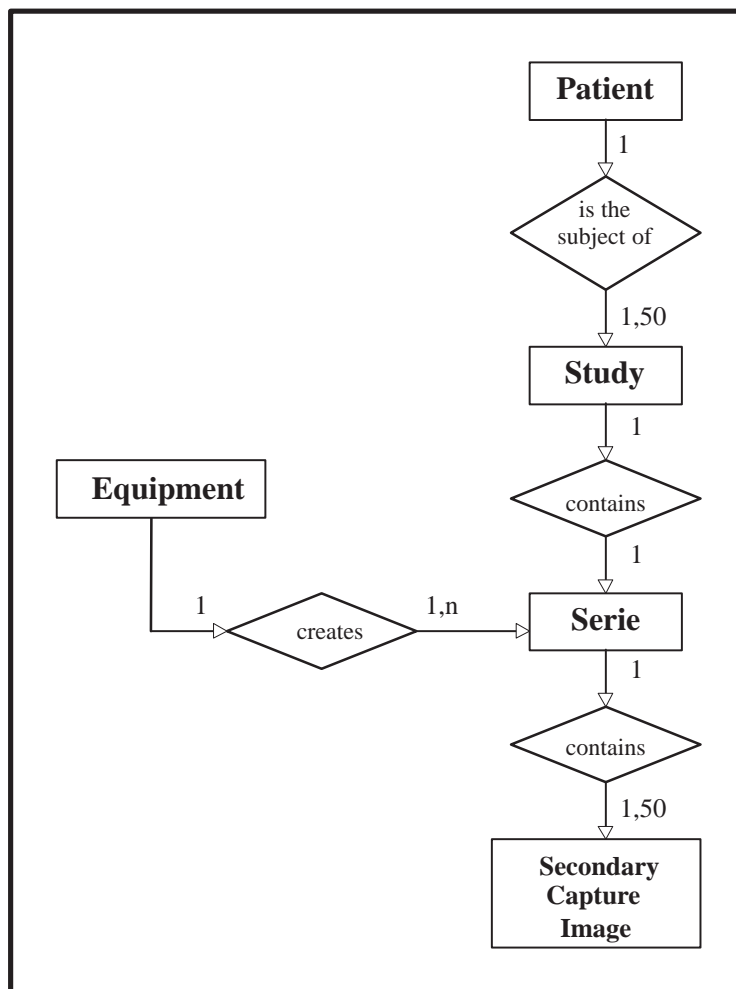

The Entity-Relationship diagram for the SC Image interoperability schema is shown in Illustration 4-1. The following diagrammatic convention is established to represent the information organisation :

- each entity is represented by a rectangular box
- each relationship is represented by a diamond shaped box
- the fact that a relationship exists between two entities is depicted by lines connecting the corresponding entity boxes to the relationship boxes.

The relationships are fully defined with the maximum number of possible entities in the relationship shown.

#### 4-2-1

### Entities Description

Refer to DICOM Standard Part 3 (Information Object Definitions) for a description of each of the entities contained within the Secondary Capture Image Information Object Definition.

4-2-2 **DLX Mapping of DICOM entities**

DICOM entities map to the DLX entities in respect to the following :

DICOM	DLX
Patient Entity	Patient Entity
Study Entity	Examination Entity
Serie Entity	no match, there is a one to one relationship between DICOM Study and Serie
Secondary Image Entity	Photo Entity

4-3 **SC IMAGE IOD MODULE TABLE**

Within an entity of the DICOM v3.0 XRAY Angio Image Information Object Definition, attributes are grouped into related set of attributes. A set of related attributes is termed a module. A module facilitates the understanding of the semantics concerning the attributes and how the attributes are related with each other. A module grouping does not infer any encoding of information into datasets.

Table 5-2 identifies the defined modules within the entities which comprise the DICOM v3.0 XRAY Angio Image Information object Definition. Modules are identified by Module Name.

See DICOM v3.0 Part 3 for a complete definition of the entities, modules, and attributes.

**Table 4.2**  
**SC Image Information Object Definition (IOD) Module Table**

IE	Module Name	Reference
Patient	Patient	5.3.1.1
Study	General Study	5.3.2.1
	Patient Study	5.3.2.2
Series	General Series	5.3.3.1
	SC Equipment	5.3.4.1
Image	General Image	5.3.5.1
	Image Pixel	5.3.5.2
	Overlay Plane	5.3.5.3
	SOP Common	5.3.5.4

4-4 **MODULE LIBRARY**

Please refer to DICOM v3.0 Standard Part 3 (Information Object Definition) for a description of each of the entities and modules contained within the SC Information Object.

Modules contain also **type 3 Private elements**.

See DICOM v3.0 Part 3 for a complete definition of the entities, modules, and attributes.

**4-4-1 Patient Entity Module****4-4-1-1 Patient Module**

Attribute Name	Element Tag	TP	Notes
Patient's Name	0010, 0010	2	
Patient ID	0010, 0020	2	
Patient's Birth Date	0010, 0030	2	No value, Zero length
Patient's Sex	0010, 0040	2	
Patient DOB	0011, xx01	3	Patient Date of birth in free form.

**4-4-2 Study Entity Module****4-4-2-1 General Study**

Attribute Name	Element Tag	TP	Notes
Study Instance UID	0020, 000D	1	
Study Date	0008, 0020	2	
Study Time	0008, 0030	2	
Referring Physicians' Name	0008, 0090	2	
Study ID	0020, 0010	2	
Study Description	0008, 1030	3	
Accession number	0008, 0050	2	No value, 0 length

**4-4-2-2 Patient Study**

Attribute Name	Element Tag	TP	Notes
Patient's Size	0010, 1020	3	
Patient's Weight	0010, 1030	3	
Additional Patient's History	0010, 21B0	3	

**4-4-3 Series Entity Module****4-4-3-1 General Series**

Attribute Name	Element Tag	TP	Notes
Modality	0008, 0060	1	value : XA
Series Instance UID	0020, 000E	1	
Series Number	0020, 0011	2	value : 1
Series Date	0008, 0021	3	
Series Time	0008, 0031	3	
Performing Physician's Name	0008, 1050	3	
Series Description	0008, 103E	3	
Operators' Name tt	0008, 1070	3	
Patient position	0008, 5100	2C	No value, Zero length

REV 1

Conformance Statement 2142506-100

**4-4-4 Equipment Entity Module****4-4-4-1 SC Equipment Module**

Attribute Name	Element Tag	TP	Notes
Conversion Type	0008, 0064	1	WSD
Modality	0008, 0060	3	XA
Secondary Capture Device Manufacturer	0018, 1016	3	GE MEDICAL SYSTEMS
Secondary Capture Device Manufacturer's Model Name	0018, 1018	3	DLX

**4-4-5 Image Entity Module****4-4-5-1 General Image**

Attribute Name	Element Tag	TP	Notes
Image Number	0020, 0013	2	Image number in the serie
Image Date	0008, 0023	2C	
Image Time	0008, 0033	2C	
Image Type	0008, 0008	3	DERIVED\SECONDARY, either SINGLE PLANE, FRONTAL or LATERAL
Patient Orientation	0020, 0020	2C	No value, Zero length
Referenced Image Sequence	0008, 1140	3	Used to reference the associated plane Secondary Capture in case of Biplane Acquisition
>Referenced SOP Class UID	0008, 1150	1C	1.2.840.10008.5.1.4.1.1.7
>Referenced SOP Instance UID	0008, 1155	1C	
Source Image Sequence	0008, 2112	3	used to reference the original acquisition
>Referenced SOP Class UID	0008, 1150	1C	1.2.840.10008.5.1.4.1.1.12.1
>Referenced SOP Instance UID	0008, 1155	1C	
Image comments	0020, 0040	3	

**4-4-5-2 Image Pixel**

Attribute Name	Element Tag	TP	Notes
Samples per Pixel	0028, 0002	1	1
Photometric Interpretation	0028, 0004	1	MONOCHROME1, MONOCHROME 2
Rows	0028, 0010	1	512 or 1024
Columns	0028, 0011	1	512 or 1024
Bits Allocated	0028, 0100	1	16
Bits Stored	0028, 0101	1	8
High Bit	0028, 0102	1	7
Pixel Representation	0028, 0103	1	0
Pixel Data	7FE0, 0010	1	

## 4-4-5-3 Overlay Plane Module

Attribute Name	Element Tag	TP	Notes
Rows	60nn, 0010	1	512 or 1024
Columns	60nn, 0011	1	512 or 1024
Overlay type	60nn, 0040	1	G
Origin	60nn, 0050	2	1,1
Bits Allocated	60nn, 0100	1	1
Bit Position	60nn, 0102	1	8..15
Gray Palette color lookup table descriptor	60nn, xx01	3	'1,1,8', to describe a lookup table of 1 entry, with the ovl value mapped on the 1rst entry of the lookup table, and with lookup table data coded on 8 bits (0.255). For complete description, refer to Palette color lookup table descriptor of Image pixel module (tag 0028,1101)
Gray Palette color lookup table data	60nn, xx02	3	0 for black overlay 255 for white overlay For complete description, refer to Palette color lookup table data of Image pixel module (tag 0028,1201)

## 4-4-5-4 SOP Common

Attribute Name	Element Tag	TP	Notes
SOP Class UID	0008, 0016	1	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	0008, 0018	1	
Specific Character Set	0008, 0005	1C	ISO-IR-100

## 4-5 PRIVATE DATA DICTIONARY FOR SECONDARY CAPTURE

Attribute Name	Data Element Tag	VR	VM
Private Creator PATIENT_01	0011,00xx	LO	1
Patient DOB	0011, xx01	LT	1
Private Creator LKUP_01	60nn,00xx	LO	1
Gray Palette color lookup table descriptor	60nn, xx01	LT	3
Gray Palette color lookup table data	60nn, xx02	LT	1

Attribute name	Data Element Tag	Value
Private Creator PATIENT_01	0011,00xx	DLX_PATNT_01
Private Creator LKUP_01	60nn,00xx	DLX_LKUP_01



## SECTION 5 – BASIC WORKLIST MANAGEMENT IMPLEMENTATION

### 5-0 INTRODUCTION


This section specifies the use of the Basic Worklist Management Information Objects to transfer the Worklist from the Information System to the Application Entity where the task is performed.

### 5-1 WORKLIST INFORMATION MODEL IMPLEMENTATION

This section defines the implementation of the Basic Worklist Information Object. It refers to the DICOM V3.0 Standard, Basic Worklist Management – Supplement 10 (August 11, 1995) to Part 3 (Information Object definition).

### 5-2 WORKLIST INFORMATION MODEL ENTITY – RELATIONSHIP DIAGRAM

ILLUSTRATION 5-1

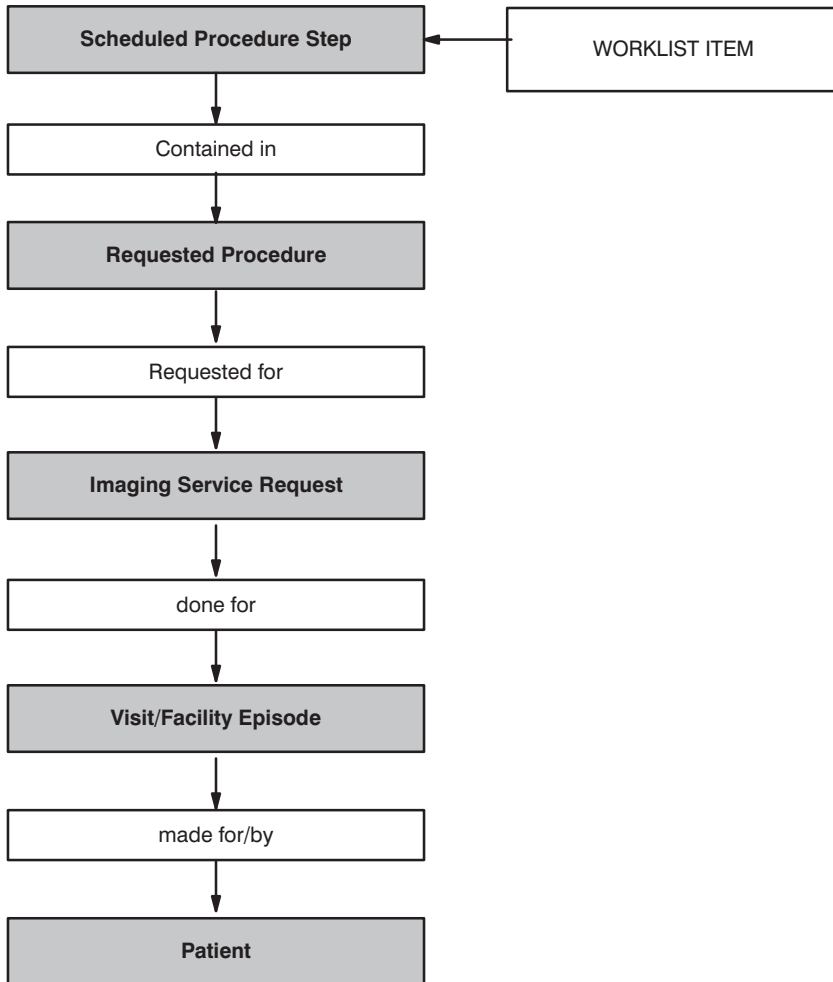

The Entity–Relationship diagram for the Basic Worklist Management interoperability schema is shown in Illustration 5–1. In this figure, the following diagrammatic convention is established to represent the information organization :

- each entity is represented by the gray rectangular box.
- each relationship is represented by the white rectangular box.
- the fact that a relationship exists between the two entities is depicted by lines connecting the corresponding entity boxes to the relationship boxes.

**5–2–1 Entities Description**

Refer to DICOM Standard Supplement 10 (August 11, 1995) to Part 3 (Information Object Definitions) for a description of the entities contained within this Information object.

**5–3 BASIC WORKLIST INFORMATION MODULE TABLE**

Within an entity of the DICOM v3.0 Basic Worklist Information Object Definition, attributes are grouped into related set of attributes. A set of related attributes is termed a module. A module facilitates the understanding of the semantics concerning the attributes and how the attributes are related with each other. A module grouping does not infer any encoding of information into data sets.

Table 2 identifies the defined modules within the entities which comprise the DICOM v3.0 Basic Worklist Management Information Object. Modules are identified by Module Name.

See DICOM v3.0 Part 3 for a complete definition of the entities, modules and attributes.

**Table 2 Basic Worklist Management Information Module Table**

IE	MODULE NAME	Reference
Patient	Patient Identification Module	para. 5–4–1–1
	Patient Demographic Module	para. 5–4–1–2
	Patient Medical Module	para. 5–4–1–3
Visit/Facility Episode	Visit Identification Module	para. 5–4–2–1
	Visit Status Module	para. 5–4–2–2
	Visit Relationship Module	para. 5–4–2–3
Imaging Service Request	Imaging Service Request Module	para. 5–4–3–1
Requested Procedure	Requested Procedure Module	para. 5–4–4–1
Scheduled Procedure Step	Scheduled Procedure Step Module	para. 5–4–5–1
	SOP Common Module	para. 5–4–5–2

**5–4 INFORMATION MODULE DEFINITIONS**

Please refer to DICOM v3.0 Standard Part 3 (Information Object Definition) and the supplements for a description of each of the entities and modules contained within the Basic Worklist Management Information Object.

Modules do not contain any **type 3 Private Elements**.

**5-4-1 Patient Entity Module****5-4-1-1 Patient Identification Module**

Attribute Name	Element Tag	Rsp TP	Notes
Patient's Name	0010, 0010	1	No value, zero length (*)
Patient ID	0010, 0020	1	No value, zero length (*)

**5-4-1-2 Patient Demographic Module**

Attribute Name	Element Tag	Rsp TP	Notes
Patient's Address	0010, 1040	3	No value, zero length (*)
Patients Telephone Numbers	0010, 2154	3	No value, zero length (*)
Patient's Birth Date	0010, 0030	2	No value, zero length (*)
Patient's Sex	0010, 0040	2	No value, zero length (*)
Patient's Size	0010, 1020	3	No value, zero length (*)
Patient's Weight	0010, 1030	3	No value, zero length (*)

**5-4-1-3 Patient Medical Module**

Attribute Name	Element Tag	Rsp TP	Notes
Additional Patient History	0010, 21B0	3	No value, zero length (*)

**5-4-2 Visit/Facility Episode Entity Module****5-4-2-1 Visit Identification Module**

Attribute Name	Element Tag	Rsp TP	Notes
Institution Name	0008, 0080	3	No value, zero length (*)
Admission ID	0038, 0010	1	No value, Zero length (*)

**5-4-2-2 Visit Status Module**

This Module is not sent as the necessary information is not available.

**5-4-2-3 Visit Relationship Module**

This Module is not sent as the necessary information is not available.

(\*) Universal Matching.

If the value specified for a key attribute in a request is zero, then all entities shall match this attribute according to its response type (i.e. Rsp Tp = 3 is optional)

**5-4-3 Imaging Service Request Entity Module****5-4-3-1 Imaging Service Request Module**

Attribute Name	Element Tag	Rsp TP	Notes
Referring Physician's Name	0008, 0090	2	No value, zero length (*)
Accession Number	0008, 0050	1	No value, zero length (*)

**5-4-4 Requested Procedure Entity Module****5-4-4-1 Requested Procedure Module**

Attribute Name	Element Tag	Rsp TP	Notes
Requested Procedure ID	0040, 1001	1	No value, zero length (*)
Study Instance UID	0020, 000D	1	No value, zero length (*)
Requested Procedure Description	0032, 1060	1C	No value, zero length (*)

**5-4-5 Scheduled Procedure Step Entity Module****5-4-5-1 Scheduled Procedure Step Module**

Attribute Name	Element Tag	Rsp TP	Notes
Scheduled Procedure Step Sequence	0040, 0100	1	No value, zero length (*)
>Scheduled Station AE title	0040, 0001	1	No value, Zero Length (*)
>Scheduled Station Name	0040, 0010	2	Possible Values : "dlx1" (**)
>Scheduled Procedure Step Start Date	0040, 0002	1	No value, Zero Length (*)
>Scheduled Procedure Step Start Time	0040, 0003	1	No value, Zero Length (*)
>Scheduled Performing Physician's Name	0040, 0006	2	No value, Zero Length (*)
>Scheduled Procedure Step ID	0040, 0009	1	No value, Zero Length (*)
>Modality	0008, 0060	1	Value = "XA" (**)

**5-4-5-2 SOP Common Module**

Attribute Name	Element Tag	Rsp TP	Notes
Specific Character Set	0008, 0005	1C	Value = "ISO_IR 100" (**)

(\*) Universal Matching.

If the value specified for a key attribute in a request is zero, then all entities shall match this attribute according to its response type (i.e. Rsp Tp = 3 is optional)

(\*\*) This means that matching is requested upon the provided value.