



GE Medical Systems



GE Medical Systems
Information Technologies

gemedical.com

Technical Publications

Direction **DCM-1030-001/00-002**
Revision **6.1.1**

Centricity Radiology RA 600 V6.1 CONFORMANCE STATEMENT for DICOM V3.0

Copyright© 1997-2003 By General Electric Co.

Do not duplicate

TABLE OF CONTENTS

| | | |
|---------|----------------------------------------------------------------------------|----|
| 1 | Introduction | 5 |
| 1.1 | Scope and Field of Application | 5 |
| 1.2 | References..... | 9 |
| 1.3 | Definitions | 9 |
| 1.4 | Symbols and Abbreviations | 9 |
| 1.5 | Revision History | 9 |
| 1.6 | Important Considerations for the Reader..... | 10 |
| 1.7 | Acknowledgment of Trade Names | 10 |
| 2 | IMPLEMENTATION MODEL..... | 11 |
| 2.1 | Application Data Flow Diagram..... | 11 |
| 2.2 | Functional Definitions of Application Entities..... | 12 |
| 2.3 | Sequencing of Real World Activities..... | 12 |
| 3 | APPLICATION ENTITY SPECIFICATIONS..... | 13 |
| 3.1 | Centricity Radiology RA 600 DICOM services AE Specifications | 13 |
| 3.1.1 | Association Establishment Policies..... | 15 |
| 3.1.1.1 | General | 15 |
| 3.1.1.2 | Number of Associations | 15 |
| 3.1.1.3 | Synchronous Nature | 15 |
| 3.1.1.4 | Implementation Identifying Information..... | 15 |
| 3.1.2 | Association Initiation Policy | 16 |
| 3.1.2.1 | Send Images to a Remote System..... | 17 |
| 3.1.2.2 | Query a Remote Database..... | 19 |
| 3.1.2.3 | Retrieve from a Remote System | 21 |
| 3.1.2.4 | Print to a remote Laser Imager..... | 22 |
| 3.1.2.5 | Retrieve a Modality Worklist from a Remote System | 27 |
| 3.1.2.6 | Send Modality Performed Procedure Step Messages to a Remote System..... | 29 |
| 3.1.2.7 | Verify the Committed Storage of Images on a Remote System | 33 |
| 3.1.2.8 | Convey a Study Status Change to a Remote System..... | 34 |
| 3.1.2.9 | Request a Study Status Change from a Remote System | 34 |
| 3.1.3 | Association Acceptance Policy | 36 |
| 3.1.3.1 | Verify Communication with a Remote System..... | 36 |
| 3.1.3.2 | Receive Images from a Remote System | 37 |
| 3.1.3.3 | Query the Centricity Radiology RA 600 Database | 40 |
| 3.1.3.4 | Retrieve from the Centricity Radiology RA 600 Database..... | 44 |
| 3.1.3.5 | Commit Storage of Images in the Centricity Radiology RA 600 Database | 45 |
| 3.1.3.6 | Receive a Study Status Change Request from a remote system..... | 47 |
| 3.1.3.7 | Receive a Study Status Change Event from a remote system..... | 48 |
| 3.2 | Centricity Radiology RA 600 DICOM Media Server AE..... | 49 |

| | | |
|----------|-------------------------------------------------------------------|----|
| 3.2.1 | Implementation Model..... | 49 |
| 3.2.1.1 | Application Data Flow Diagram..... | 49 |
| 3.2.1.2 | File Meta Information Options..... | 49 |
| 3.2.2 | AE Specifications..... | 50 |
| 3.2.2.1 | Centricity Radiology RA 600 Application Entity Specification..... | 50 |
| 3.2.2.2 | Real-World Activities..... | 51 |
| 3.2.3 | Character Sets..... | 57 |
| 4 | COMMUNICATION PROFILE..... | 58 |
| 4.1 | Supported Communication Stacks..... | 58 |
| 4.2 | OSI Stack..... | 58 |
| 4.3 | TCP/IP Stack..... | 58 |
| 4.3.1 | Physical Media Support..... | 58 |
| 4.4 | Point-to-Point Stack..... | 58 |
| 5 | EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS..... | 59 |
| 5.1 | Standard Extended / Specialized / Private SOPs..... | 59 |
| 5.1.1 | GSPS objects referring to colour images..... | 59 |
| 5.1.2 | Collage IOD..... | 59 |
| 5.1.2.1 | SOP Class UID..... | 59 |
| 5.2 | Private Transfer Syntaxes..... | 59 |
| 5.3 | Private Tags..... | 60 |
| 5.3.1 | Private tags created and used in GSPS objects..... | 60 |
| 5.3.2 | Private tags, read from IODs..... | 60 |
| 5.3.3 | Private tags supported by the Query SCP (Study Level)..... | 61 |
| 6 | CONFIGURATION..... | 62 |
| 6.1 | AE Title/Presentation Address Mapping..... | 62 |
| 6.2 | Configurable Parameters..... | 62 |
| 7 | SUPPORT OF EXTENDED CHARACTER SETS..... | 63 |
| Annex A: | GE Medical Systems Private Uncompressed Application Profile..... | 64 |
| A.1 | CLASS AND PROFILE IDENTIFICATION..... | 64 |
| A.2 | CLINICAL CONTEXT..... | 64 |
| A.2.1 | ROLES AND SERVICE CLASS OPTIONS SECTION..... | 64 |
| A.3 | GENERAL CLASS PROFILE..... | 65 |
| A.3.1 | SOP CLASSES AND TRANSFER SYNTAXES..... | 65 |
| A.3.2 | PHYSICAL MEDIA AND MEDIA FORMATS..... | 65 |
| A.3.3 | DIRECTORY INFORMATION IN DICOMDIR..... | 66 |
| Annex B: | GE Medical Systems Private Compressed Application Profile..... | 67 |
| B.1 | CLASS AND PROFILE IDENTIFICATION..... | 67 |

| | | |
|----------|-----------------------------------------------------------|----|
| B.2 | CLINICAL CONTEXT | 67 |
| B.2.1 | ROLES AND SERVICE CLASS OPTIONS SECTION | 67 |
| B.3 | GENERAL CLASS PROFILE | 68 |
| B.3.1 | SOP CLASSES AND TRANSFER SYNTAXES | 68 |
| B.3.2 | PHYSICAL MEDIA AND MEDIA FORMATS | 68 |
| B.3.3 | DIRECTORY INFORMATION IN DICOMDIR | 69 |
| Annex C: | GE Medical Systems Private Cardiac Exchange Profile | 70 |
| C.1 | CLASS AND PROFILE IDENTIFICATION | 70 |
| C.2 | CLINICAL CONTEXT | 70 |
| C.2.1 | ROLES AND SERVICE CLASS OPTIONS SECTION | 70 |
| C.3 | GENERAL CLASS PROFILE | 70 |
| C.3.1 | SOP CLASSES AND TRANSFER SYNTAXES | 70 |
| C.3.2 | PHYSICAL MEDIA AND MEDIA FORMATS | 71 |
| C.3.3 | DIRECTORY INFORMATION IN DICOMDIR | 71 |
| C.4 | SPECIFIC APPLICATION PROFILES | 71 |
| C.4.1 | PRI-GEMS-CVIS-EXCHANGE | 71 |
| Annex D: | GE Medical Systems Private Cardiac Archive Profile | 72 |
| D.1 | CLASS AND PROFILE IDENTIFICATION | 72 |
| D.2 | CLINICAL CONTEXT | 72 |
| D.2.1 | ROLES AND SERVICE CLASS OPTIONS SECTION | 72 |
| D.3 | GENERAL CLASS PROFILE | 72 |
| D.3.1 | SOP CLASSES AND TRANSFER SYNTAXES | 72 |
| D.3.2 | PHYSICAL MEDIA AND MEDIA FORMATS | 73 |
| D.3.3 | DIRECTORY INFORMATION IN DICOMDIR | 73 |
| D.4 | SPECIFIC APPLICATION PROFILES | 73 |
| D.4.1 | PRI-GEMS-CVIS-ARCHIVE | 73 |

1 Introduction

1.1 Scope and Field of Application

This document is the DICOM Conformance Statement for version 6.1 of the Centricity Radiology RA 600 product line of GE Medical Systems IT. The purpose of this document is to describe how the Centricity Radiology RA 600 product suite collaborates in a DICOM network with other medical imaging applications that conform to the DICOM 3.0 standard.


1.2 OVERVIEW

This DICOM Conformance Statement is divided into Sections as described below:

- **Section 1 (Introduction)**, which describes the overall structure, intent, and references for this Conformance Statement
- **Section 2 (Implementation Model)**, which describes the data flow fro DICOM associations
- **Section 3 (Application Entity Specifications)**, which describes the DICOM network services and association policies for initiation and acceptance. Furthermore the DICOM Media Server properties are described.
- **Section 4 (Communication Profile)**, which describes the communication stack behavior.
- **Section 5 (Extensions / Specializations / Privatizations)**, which describes the private features of Centricity Radiology RA 600, which are public available.
- **Section 6 (Configuration)**, which describes the configurable parameters for Centricity Radiology RA 600 that have influence on the DICOM behavior.
- **Section 7 (Extended Charact Sets)**, which describes the Character sets supported by Centricity Radiology RA 600.

1.3 OVERALL DICOM CONFORMANCE STATEMENT DOCUMENT STRUCTURE

The Documentation Structure of the GEMS Conformance Statements and their relationship with the DICOM v3.0 Conformance Statements is shown in the Illustration below.

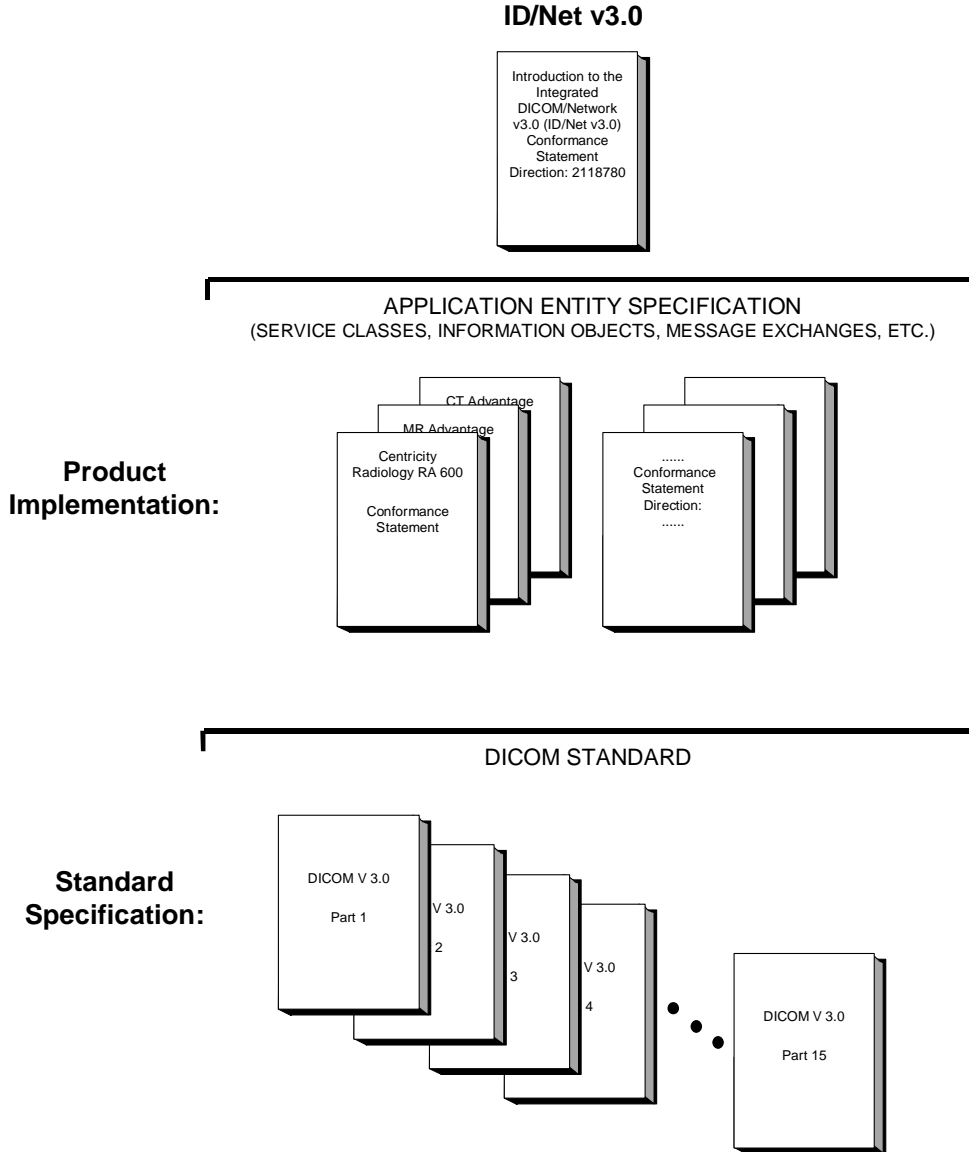

This document specifies the DICOM v3.0 implementation. It is entitled:
Centricity Radiology RA 600 V6.1
Conformance Statement for DICOM v3.0
Direction DCM-1030-001/00-002

This DICOM Conformance Statement documents the DICOM v3.0 Conformance Statement and Technical Specification required to interoperate with the GEMS network interface.

Introductory information, which is applicable to all GEMS Conformance Statements, is described in the document:

*Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0)
Conformance Statement
Direction: 2118780.*

This Introduction familiarizes the reader with DICOM terminology and general concepts. It should be read prior to reading the individual products' GEMS Conformance Statements. The GEMS Conformance Statement, contained in this document, also specifies the Lower Layer communications, which it supports (e.g., TCP/IP). However, the Technical Specifications are defined in the DICOM v3.0 Part 8 standard.

For more information including Network Architecture and basic DICOM concepts, please refer to the Introduction.

For the convenience of software developers, there is "collector" Direction available. By ordering the collector, the Introduction described above and all of the currently published GEMS Product Conformance Statements will be received. The collector Direction is:

*ID/Net v3.0 Conformance Statements
Direction: 2117016*

For more information regarding DICOM v3.0, copies of the Standard may be obtained by written request or phone by contacting:

NEMA Publication
1300 North 17th Street
Suite 1847
Rosslyn, VA 22209
USA
Phone: (703) 841-3200

1.4 INTENDED AUDIENCE

The reader of this document is concerned with software design and/or system integration issues. It is assumed that the reader of this document is familiar with the DICOM v3.0 Standards and with the terminology and concepts that are used in those Standards. If readers are unfamiliar with DICOM v3.0 terminology they should first refer to the document listed below, then read the DICOM v3.0 Standard itself, prior to reading this DICOM Conformance Statement document.

*Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0)
Conformance Statement
Direction: 2118780*

1.5 SCOPE AND FIELD OF APPLICATION

It is the intent of this document, in conjunction with the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*, to provide an unambiguous specification for GEMS implementations. This specification, called a Conformance Statement, includes a DICOM v3.0 Conformance Statement and is necessary to ensure proper processing and interpretation of GEMS medical data exchanged using DICOM v3.0. The GEMS Conformance Statements are available to the public. The reader of this DICOM Conformance Statement should be aware that different GEMS devices are capable of using different Information Object Definitions. For example, a GEMS

CT Scanner may send images using the CT Information Object, MR Information Object, Secondary Capture Object, etc.

Included in this DICOM Conformance Statement are the Module Definitions, which define all data elements, used by this GEMS implementation. If the user encounters unspecified private data elements while parsing a GEMS Data Set, the user is well advised to ignore those data elements (per the DICOM v3.0 standard). Unspecified private data element information is subject to change without notice. If, however, the device is acting as a "full fidelity storage device", it should retain and re-transmit all of the private data elements that are sent by GEMS devices.

1.6 IMPORTANT REMARKS

The use of these DICOM Conformance Statements, in conjunction with the DICOM v3.0 Standards, is intended to facilitate communication with GE imaging equipment. However, **by itself, it is not sufficient to ensure that inter-operation will be successful.** The **user (or user's agent)** needs to proceed with caution and address at least four issues:

- **Integration** - The integration of any device into an overall system of interconnected devices goes beyond the scope of standards (DICOM v3.0), and of this introduction and associated DICOM Conformance Statements when interoperability with non-GE equipment is desired. The responsibility to analyze the applications requirements and to design a solution that integrates GE imaging equipment with non-GE systems is the **user's** responsibility and should not be underestimated. The **user** is strongly advised to ensure that such an integration analysis is correctly performed.
- **Validation** - Testing the complete range of possible interactions between any GE device and non-GE devices, before the connection is declared operational, should not be overlooked. Therefore, the **user** should ensure that any non-GE provider accepts full responsibility for all validation required for their connection with GE devices. This includes the accuracy of the image data once it has crossed the interface between the GE imaging equipment and the non-GE device and the stability of the image data for the intended applications.

Such a validation is required before any clinical use (diagnosis and/or treatment) is performed. It applies when images acquired on GE imaging equipment are processed/displayed on a non-GE device, as well as when images acquired on non-GE equipment is processed/displayed on a GE console or workstation.
- **Future Evolution** - GE understands that the DICOM Standard will evolve to meet the user's growing requirements. GE is actively involved in the development of the DICOM v3.0 Standard. DICOM v3.0 will incorporate new features and technologies and GE may follow the evolution of the Standard. The GEMS protocol is based on DICOM v3.0 as specified in each DICOM Conformance Statement. Evolution of the Standard may require changes to devices that have implemented DICOM v3.0. **In addition, GE reserves the right to discontinue or make changes to the support of communications features (on its products) reflected on by these DICOM Conformance Statements.** The user should ensure that any non-GE provider, which connects with GE devices, also plans for the future evolution of the DICOM Standard. Failure to do so will likely result in the loss of function and/or connectivity as the DICOM Standard changes and GE Products are enhanced to support these changes.
- **To be informed of the evolution of the implementation described in this document, the User is advised to regularly check the GE Internet Server, accessible via anonymous ftp (GE Internet Server Address: ftp.med.ge.com, 192.88.230.11).**

- **Interaction** - It is the sole responsibility of the **non-GE provider** to ensure that communication with the interfaced equipment does not cause degradation of GE imaging equipment performance and/or function.

1.7 REFERENCES

A list of references, which is applicable to all GEMS Conformance Statements, is included in the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*.

1.8 DEFINITIONS

A set of definitions, which is applicable to all GEMS Conformance Statements, is included in the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*.

1.9 SYMBOLS AND ABBREVIATIONS

A list of symbols and abbreviations, which is applicable to all GEMS Conformance Statements, is included in the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*.

1.10 Revision History

| Version | Date | Description |
|-------------|----------------|-------------------------------------------------------|
| Preliminary | September 1995 | Preliminary version |
| 1.0 | October 1995 | First official version |
| 1.1 (Draft) | July 1996 | First revision (Draft) |
| 2.0 | November 1996 | Second official version |
| 2.1 | June 1997 | Updated for RadWorks 2.1 release |
| 2.1a | August 1997 | Final (minor) update for RadWorks 2.1 release |
| 4.0 | November 1998 | Updated for RadWorks 4.0 release |
| 5.0 | 5 August 1999 | Updated for RadWorks 5.0 release |
| 5.1 | September 2000 | Updated for RadWorks 5.1 release |
| 6.0 | 13 May 2002 | Update for Centricity Radiology RA 600 6.0 M4 Release |
| 6.1 | January 2003 | Update for Centricity Radiology RA 600 6.1 M4 Release |
| 6.1.1 | 1 May 2003 | Update for Centricity Radiology RA 600 6.1 SR2 |

1.11 Important Considerations for the Reader

This DICOM Conformance Statement by itself is not sufficient to guarantee successful connectivity between Centricity Radiology RA 600 and equipment from other vendors. The following considerations should be made:

- The integration of equipment from different vendors (including GE Medical Systems) goes beyond the scope of the DICOM 3.0 standard and the DICOM Conformance Statements from GE Medical Systems and other vendors. It is the responsibility of the user (or user's agent) to assess the application requirements and to design a solution that integrates GE Medical Systems equipment with equipment from other vendors.
- When the comparison of this DICOM Conformance Statement with a DICOM Conformance Statement from another vendor indicates that connectivity should be possible it is the responsibility of the user (or user's agent) to verify this by carrying out validation tests and to check whether all required functionality is met.
- With regard to the future evolution of the DICOM 3.0 standard GE Medical Systems reserves the right to make changes to the Centricity Radiology RA 600 architecture described in this document. The user (or user's agent) should ensure that any equipment connected via DICOM to GE Medical Systems IT equipment also follows the future evolution of the DICOM 3.0 standard. Failure to do so may result in (partial) loss of connectivity.

1.12 Acknowledgment of Trade Names

All trade names mentioned in this document are recognized.


Centricity Radiology RA 600 is a registered trademark of GE Medical Systems

2 IMPLEMENTATION MODEL

The Centricity Radiology RA 600 DICOM services are implemented as three separate processes that share a single Application Entity Title. Currently all three processes can all initiate associations with remote application entities while one can accept associations from remote Application Entities as well. In addition the Centricity Radiology RA 600 front-end application can initiate (but not accept¹) DICOM associations with remote application entities.

2.1 Application Data Flow Diagram

The Implementation Model for the Centricity Radiology RA 600 DICOM services is depicted below:

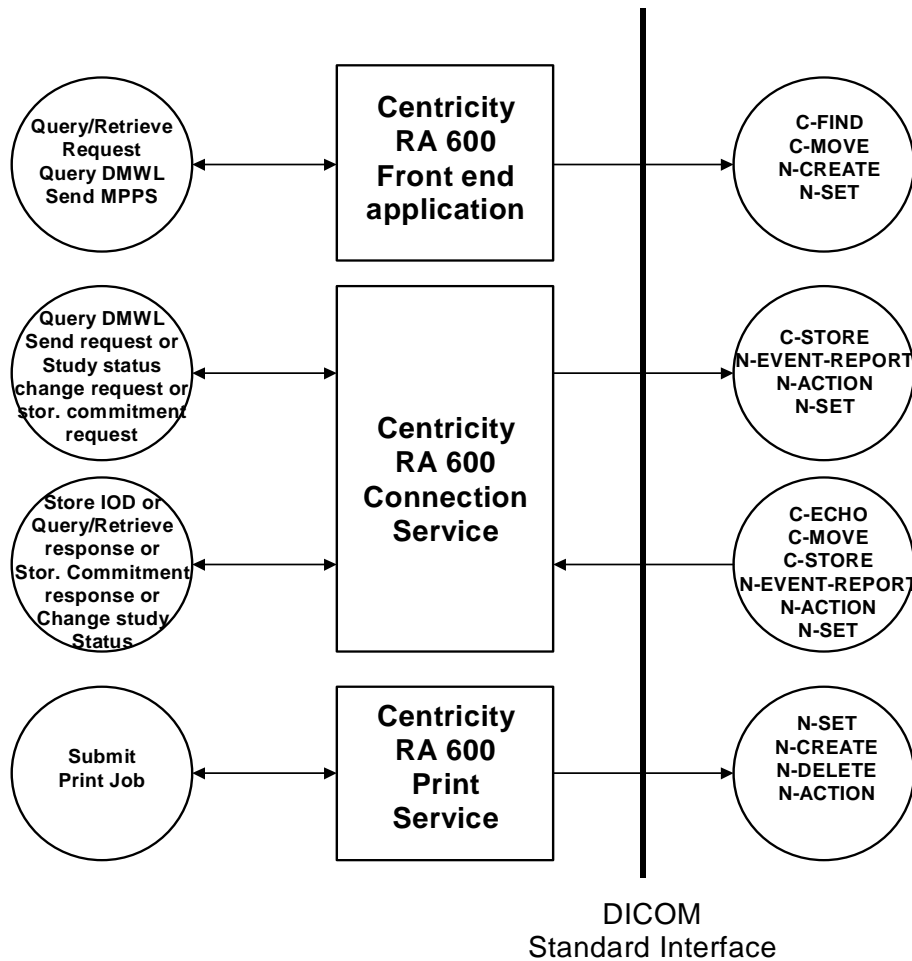

The Centricity Radiology RA 600 DICOM services are implemented as three separate Windows services that run as background processes. They are started automatically during system start-up and will remain active until shutdown. This means that requests for, e.g.,

¹ SCP behavior is implemented in the Connection Service and not by the front-end application or Database Service. In other words: the Connection Service is the single point of entry for incoming DICOM connectivity and it's always alive when the system is turned on. The Centricity Radiology RA 600 front-end application can be shut down without influencing incoming DICOM connectivity.

image storage can be accepted at all times when the system is up and running regardless of whether the Centricity Radiology RA 600 application is active or not.

The Centricity Radiology RA 600 Connection Service is responsible for image reception and transmission in addition to accepting requests for database queries and retrieves. It maintains logs of all studies that entered and left the system. It can perform scheduled image transfers to remote Application Entities at all times.

The Centricity Radiology RA 600 front-end application issues queries to remote DICOM databases and initiates import requests. Please note that the destination of imports is the Centricity Radiology RA 600 Connection Service.

The Centricity Radiology RA 600 Print Service is responsible for managing print job queues for one or more printers or laser imagers. It supports several protocols of which the DICOM standard is one.

The Centricity Radiology RA 600 Database and Connection Services are integral parts of a Centricity Radiology RA 600 installation. Please note that the Print Service as a whole is an optional component of a Centricity Radiology RA 600 installation.

In addition to the Storage SOP Class support for networking, Centricity Radiology RA 600 also supports the Media Storage Service Class for the Interchange of images as a File Set Reader (FSR) and File Set Creator (FSC). FSR is a standard feature and FSC is an optional feature. See section 3.2 for further details.

2.2 Functional Definitions of Application Entities

The Application Entity of the Centricity Radiology RA 600 Connection Service acts as an SCU for the storage and storage commitment SOP classes and as an SCP for verification, storage, query, retrieve, and storage commitment SOP classes. In specific situations Centricity Radiology RA 600 Connection Service may act as an SCU for DICOM Modality Worklists

The Application Entity of the Centricity Radiology RA 600 front-end application acts as an SCU for the query and retrieve SOP classes. In specific situations the Centricity Radiology RA 600 front-end application may act as an SCU for DICOM Modality Worklists SOP class, and as an SCU for the Modality Performed Procedure Step SOP class.

The Application Entity of the Centricity Radiology RA 600 Print Service acts as an SCU for the basic grayscale and color print management meta SOP classes, and optionally the Print Job and Basic Annotation Box SOP classes.

2.3 Sequencing of Real World Activities

Not applicable.

3 APPLICATION ENTITY SPECIFICATIONS

3.1 Centricity Radiology RA 600 DICOM services AE Specifications

The Centricity Radiology RA 600 DICOM services provide support for the following DICOM V3.0 SOP Classes, both as an SCU and an SCP:

| SOP Classes as SCU and SCP | |
|------------------------------------------------|--------------------------------|
| SOP Class Name | SOP Class UID |
| Detached Study Management | 1.2.840.10008.3.1.2.3.1 |
| Patient Root Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.1.1 |
| Patient Root Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.1.2 |
| Study Root Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.2.1 |
| Study Root Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.2.2 |
| Patient/Study Only Query/Retrieve Model – FIND | 1.2.840.10008.5.1.4.1.2.3.1 |
| Patient/Study Only Query/Retrieve Model – MOVE | 1.2.840.10008.5.1.4.1.2.3.2 |
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 |
| CR Image | 1.2.840.10008.5.1.4.1.1.1 |
| DX Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.1 |
| DX Image (Process) | 1.2.840.10008.5.1.4.1.1.1.1.1 |
| DX Mammography Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.2 |
| DX Mammography Image (Process) | 1.2.840.10008.5.1.4.1.1.1.2.1 |
| DX Intra-oral Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.3 |
| DX Intra-oral Image (Process) | 1.2.840.10008.5.1.4.1.1.1.3.1 |
| CT Image | 1.2.840.10008.5.1.4.1.1.2 |
| US Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.3 |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 |
| NM Image (Retired) | 1.2.840.10008.5.1.4.1.1.5 |
| US Image (Retired) | 1.2.840.10008.5.1.4.1.1.6 |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 |
| Multi-Frame Single Bit SC Image | 1.2.840.10008.5.1.4.1.1.7.1 |
| Multi-Frame Grayscale Byte SC Image | 1.2.840.10008.5.1.4.1.1.7.2 |
| Multi-Frame Grayscale Word SC Image | 1.2.840.10008.5.1.4.1.1.7.3 |
| Multi-Frame True Color SC Image | 1.2.840.10008.5.1.4.1.1.7.4 |
| Standalone Overlay | 1.2.840.10008.5.1.4.1.1.8 |
| Standalone Curve | 1.2.840.10008.5.1.4.1.1.9 |
| Standalone Modality LUT | 1.2.840.10008.5.1.4.1.1.10 |
| Standalone VOI LUT | 1.2.840.10008.5.1.4.1.1.11 |
| Grayscale Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.1 |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 |
| XF Image | 1.2.840.10008.5.1.4.1.1.12.2 |
| NM Image | 1.2.840.10008.5.1.4.1.1.20 |
| VL Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.1 |
| VL Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.2 |
| VL Endoscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.1 |
| VL Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.2 |
| VL Slide-Coordinates Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.3 |
| VL Photographic Image | 1.2.840.10008.5.1.4.1.1.77.1.4 |
| Basic Text Structured Reports | 1.2.840.10008.5.1.4.1.1.88.11 |
| Enhanced Structured Reports | 1.2.840.10008.5.1.4.1.1.88.22 |
| Comprehensive Structured Reports | 1.2.840.10008.5.1.4.1.1.88.33 |
| Key Object Selection | 1.2.840.10008.5.1.4.1.1.88.59 |
| PET Image | 1.2.840.10008.5.1.4.1.1.128 |
| Standalone PET Curve | 1.2.840.10008.5.1.4.1.1.129 |
| RT Image | 1.2.840.10008.5.1.4.1.1.481.1 |
| RT Dose | 1.2.840.10008.5.1.4.1.1.481.2 |
| RT Structure Set | 1.2.840.10008.5.1.4.1.1.481.3 |
| RT Beams Treatment Record | 1.2.840.10008.5.1.4.1.1.481.4 |
| RT Plan | 1.2.840.10008.5.1.4.1.1.481.5 |
| RT Brachy Treatment Record | 1.2.840.10008.5.1.4.1.1.481.6 |
| RT Treatment Summary Record | 1.2.840.10008.5.1.4.1.1.481.7 |

| SOP Classes as SCP Only | |
|-------------------------|-------------------|
| SOP Class Name | SOP Class UID |
| Verification | 1.2.840.10008.1.1 |

| SOP Classes as SCU Only | |
|--------------------------------------------|-------------------------|
| SOP Class Name | SOP Class UID |
| Verification | 1.2.840.10008.1.1 |
| Basic Grayscale Print Management Meta | 1.2.840.10008.5.1.1.9 |
| Basic Color Print Management Meta | 1.2.840.10008.5.1.1.18 |
| Print Job | 1.2.840.10008.5.1.1.14 |
| Basic Annotation Box | 1.2.840.10008.5.1.1.15 |
| Modality Worklist Information Model - FIND | 1.2.840.10008.5.1.4.31 |
| Modality Performed Procedure Step | 1.2.840.10008.3.1.2.3.3 |

Though Centricity Radiology RA 600 is able to receive many SOP classes, not all SOP classes can be completely visualized. The following features concern visualization of IODs:

- The DICOM information of all storage IODs can be displayed in raw or formatted form, including private data
- Image type Storage IODs can be displayed with their image data, when their Photometric interpretation is one of the types “MONochrome1”, “MONochrome2”, “RGB”, “PALETTE COLOR”, “YBR_FULL” and “YBR_FULL_422”.
- Grayscale Softcopy Presentation State IODs can be applied to studies or displayed with their referenced images completely, except for the following sub-features:
 - Masks
 - Bitmap Display Shutters
 - Overlay Planes
 - Overlay/Curve Activation
- Basic Structured Reports IODs can be displayed, including resolving Image UID references. Enhanced and Comprehensive Structured Reports will be displayed likewise, but their enhanced features like SCOORD Value Types will not be resolved graphically. Their complete contents will be displayed though in a character type way.
- Key Object Note IODs can be either displayed with their images or applied to the images currently displayed. In both cases Centricity Radiology RA 600 only supports references to images of the same study the key note object IOD is part of. ‘Foreign’ references are just ignored.

3.1.1 Association Establishment Policies

3.1.1.1 General

The configuration of the Centricity Radiology RA 600 DICOM services in the Windows Registry shall define such parameters as Application Entity title, host name, and port number that are shared by the Connection, Database and Print Services. They offer a (configurable) maximum PDU size of 4 MB (4194304 bytes) upon association initiation and on associations initiated by remote applications.

3.1.1.2 Number of Associations

The Centricity Radiology RA 600 Connection Service supports multiple associations both as an SCU² and SCP. The maximum number of simultaneous associations that the Connection Service will support as an SCP is configurable and it defaults to 4.

The Centricity Radiology RA 600 front-end application supports multiple associations as an SCU for query and retrieve to different SCPs.

The Centricity Radiology RA 600 Print Service SCU will queue its DICOM print jobs in a way that it only establishes one association at a time.

3.1.1.3 Synchronous Nature

The Centricity Radiology RA 600 DICOM services do not support asynchronous operations and will not perform asynchronous window negotiation.

3.1.1.4 Implementation Identifying Information

The Implementation Class UID is: 1.2.528.1.1001.2.20020916.1
The version name is: AMI_DICOM01_2

² When the Connection Service is actively sending data, it will effectively use one single association at a time. Multiple simultaneous associations as an SCU may occur when the Connection Service is processing a C-Move request as an SCP.

3.1.2 Association Initiation Policy

The Centricity Radiology RA 600 Connection Service initiates associations for the following activities:

- The Centricity Radiology RA 600 user wants to send images or other IODs from the local Centricity Radiology RA 600 database to a remote system.
- The Centricity Radiology RA 600 user wants to request storage commitment after images from the local Centricity Radiology RA 600 database have been transmitted to a remote system.
- The Centricity Radiology RA 600 user wants to convey a study status change to a remote system
- The Centricity Radiology RA 600 user wants a remote system to change the study status for a certain study.

The Centricity Radiology RA 600 front-end application initiates associations for the following activities:

- The Centricity Radiology RA 600 user wants to query the contents of a remote database on a Patient, Study, Series or Instance level.
- The Centricity Radiology RA 600 user wants to retrieve studies, series, images or other IODs from a remote database into the local Centricity Radiology RA 600 database.
- The Centricity Radiology RA 600 user wants to retrieve a Modality Worklist from an external Modality Worklist Provider
- The Centricity Radiology RA 600 user wants to send a Modality Performed Procedure Step success message to indicate that a DICOM Modality Worklist item was handled and resulted in a study, ready for reading by the radiologist (using the optional Quality Control module).
- The Centricity Radiology RA 600 user wants to send a Modality Performed Procedure Step failure message to indicate that a DICOM Modality Worklist item will not be handled (using the optional Quality Control module).

The Centricity Radiology RA 600 Print Service initiates associations for the following activities:

- The Centricity Radiology RA 600 user wants to print images to a laser imager.

3.1.2.1 Send Images to a Remote System

3.1.2.1.1 Associated Real World Activity

The user of the Centricity Radiology RA 600 system makes a selection of one or more studies and series in the local Database and subsequently presses the Send button which will initiate the transfer of images from the local database of Centricity Radiology RA 600 to the remote system.

3.1.2.1.2 Proposed Presentation Contexts

| Presentation Context Table for Send To Remote System | | | | |
|------------------------------------------------------|--------------------------------|----------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | Role | Extended Negotiation |
| Name | UID | | | |
| CR Image | 1.2.840.10008.5.1.4.1.1.1 | See UID list A below | SCU | None |
| DX Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.1 | See UID list A below | SCU | None |
| DX Image (Process) | 1.2.840.10008.5.1.4.1.1.1.1.1 | See UID list A below | SCU | None |
| DX Mammography Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.2 | See UID list A below | SCU | None |
| DX Mammography Image (Process) | 1.2.840.10008.5.1.4.1.1.1.2.1 | See UID list A below | SCU | None |
| DX Intra-oral Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.3 | See UID list A below | SCU | None |
| DX Intra-oral Image (Process) | 1.2.840.10008.5.1.4.1.1.1.3.1 | See UID list A below | SCU | None |
| CT Image | 1.2.840.10008.5.1.4.1.1.2 | See UID list A below | SCU | None |
| US Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.3 | See UID list A below | SCU | None |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 | See UID list A below | SCU | None |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 | See UID list A below | SCU | None |
| NM Image (Retired) | 1.2.840.10008.5.1.4.1.1.5 | See UID list A below | SCU | None |
| US Image (Retired) | 1.2.840.10008.5.1.4.1.1.6 | See UID list A below | SCU | None |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 | See UID list A below | SCU | None |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 | See UID list A below | SCU | None |
| Multi-Frame Single Bit SC Image | 1.2.840.10008.5.1.4.1.1.7.1 | See UID list A below | SCU | None |
| Multi-Frame Grayscale Byte SC Image | 1.2.840.10008.5.1.4.1.1.7.2 | See UID list A below | SCU | None |
| Multi-Frame Grayscale Word SC Image | 1.2.840.10008.5.1.4.1.1.7.3 | See UID list A below | SCU | None |
| Multi-Frame True Color SC Image | 1.2.840.10008.5.1.4.1.1.7.4 | See UID list A below | SCU | None |
| Standalone Overlay | 1.2.840.10008.5.1.4.1.1.8 | See UID list B below | SCU | None |
| Standalone Curve | 1.2.840.10008.5.1.4.1.1.9 | See UID list B below | SCU | None |
| Standalone Modality LUT | 1.2.840.10008.5.1.4.1.1.10 | See UID list B below | SCU | None |
| Standalone VOI LUT | 1.2.840.10008.5.1.4.1.1.11 | See UID list B below | SCU | None |
| Grayscale Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.1 | See UID list B below | SCU | None |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | See UID list A below | SCU | None |
| XF Image | 1.2.840.10008.5.1.4.1.1.12.2 | See UID list A below | SCU | None |
| NM Image | 1.2.840.10008.5.1.4.1.1.20 | See UID list A below | SCU | None |
| VL Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.1 | See UID list A below | SCU | None |
| VL Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.2 | See UID list A below | SCU | None |
| VL Endoscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.1 | See UID list A below | SCU | None |
| VL Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.2 | See UID list A below | SCU | None |
| VL Slide-Coordinates Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.3 | See UID list A below | SCU | None |
| VL Photographic Image | 1.2.840.10008.5.1.4.1.1.77.1.4 | See UID list A below | SCU | None |
| Basic Text Structured Reports | 1.2.840.10008.5.1.4.1.1.88.11 | See UID list B below | SCU | None |
| Enhanced Structured Reports | 1.2.840.10008.5.1.4.1.1.88.22 | See UID list B below | SCU | None |
| Comprehensive Structured Reports | 1.2.840.10008.5.1.4.1.1.88.33 | See UID list B below | SCU | None |
| Key Object Selection | 1.2.840.10008.5.1.4.1.1.88.59 | See UID list B below | SCU | None |
| PET Image | 1.2.840.10008.5.1.4.1.1.128 | See UID list A below | SCU | None |
| Standalone PET Curve | 1.2.840.10008.5.1.4.1.1.129 | See UID list B below | SCU | None |
| RT Image | 1.2.840.10008.5.1.4.1.1.481.1 | See UID list A below | SCU | None |
| RT Dose | 1.2.840.10008.5.1.4.1.1.481.2 | See UID list B below | SCU | None |
| RT Structure Set | 1.2.840.10008.5.1.4.1.1.481.3 | See UID list B below | SCU | None |
| RT Beams Treatment Record | 1.2.840.10008.5.1.4.1.1.481.4 | See UID list B below | SCU | None |
| RT Plan | 1.2.840.10008.5.1.4.1.1.481.5 | See UID list B below | SCU | None |
| RT Brachy Treatment Record | 1.2.840.10008.5.1.4.1.1.481.6 | See UID list B below | SCU | None |
| RT Treatment Summary Record | 1.2.840.10008.5.1.4.1.1.481.7 | See UID list B below | SCU | None |

UID List A:

| Transfer Syntaxes for Send To Remote System | |
|----------------------------------------------------------------------|------------------------|
| Name | UID |
| Implicit VR, Little Endian | 1.2.840.10008.1.2 |
| Explicit VR, Little Endian | 1.2.840.10008.1.2.1 |
| Explicit VR, Big Endian | 1.2.840.10008.1.2.2 |
| Explicit VR, Lossy JPEG 8-Bit Image Compression | 1.2.840.10008.1.2.4.50 |
| Explicit VR, Lossy JPEG 12-Bit Image Compression | 1.2.840.10008.1.2.4.51 |
| Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction | 1.2.840.10008.1.2.4.70 |
| Explicit VR, RLE Lossless compression | 1.2.840.10008.1.2.5 |
| Explicit VR, AMI Wavelet Progressive Lossy Compression | 1.2.528.1.1001.4.1.1.2 |
| Explicit VR, AMI JPEG Lossy Compression 8-bit | 1.2.528.1.1001.4.2.1.1 |
| Explicit VR, AMI JPEG Lossy Compression 12-bit | 1.2.528.1.1001.4.2.1.2 |
| Explicit VR, AMI ZLIB Lossless Compression | 1.2.528.1.1001.4.4.1 |

UID List B:

| Transfer Syntaxes for Send To Remote System | |
|---------------------------------------------|---------------------|
| Name | UID |
| Implicit VR, Little Endian | 1.2.840.10008.1.2 |
| Explicit VR, Little Endian | 1.2.840.10008.1.2.1 |
| Explicit VR, Big Endian | 1.2.840.10008.1.2.2 |

3.1.2.1.3 SOP Specific Conformance Statement for SOP Class Storage

The images stored in the local Centricity Radiology RA 600 database that are to be sent are converted from the local Centricity Radiology RA 600 DICOM 3.0 compliant format to instances of the corresponding SOP Storage class(es) and subsequently sent to the remote system.

Centricity Radiology RA 600 allows image transfers to be scheduled for specific times and has mechanisms for retrying a transfer in case that a transfer failed at an earlier time. After a configurable number of unsuccessful attempts Centricity Radiology RA 600 will mark the transfer as failed. The Centricity Radiology RA 600 system keeps a log of transfers that is viewable by the user. The log indicates the status of transfers.

Centricity Radiology RA 600 provides full (level 2) conformance as SCP of the Storage SOP class. This means that upon sending an image received via DICOM on to another DICOM compliant system it will send out all attributes that it received (this includes private attributes from other vendors).

When the user selects a DICOM Lossy JPEG transfer syntax to be used for sending a certain study to another system the study will be compressed before transmission if it was not already compressed. The attributes "Derivative Description" (0008,2111) and "Lossy Compression" (0008, 2112) will be set to specify that Lossy JPEG compression has been applied to the pixel data and this string has to be shown to the user when the images are subsequently viewed (as is done by Centricity Radiology RA 600). In the case the receiving workstation is from a 3rd party vendor it is their responsibility to display this string correctly.

If the study in the Centricity Radiology RA 600 database was stored in JPEG Lossless or Lossy format (because it was received previously with compression, or compressed before storage) the DICOM JPEG Lossless or Lossy transfer syntax will be requested in addition to and in preference of the explicit and implicit little endian transfer syntaxes. If the C-STORE SCP chooses not to use the DICOM JPEG transfer syntax, the image data will be decompressed before it will be sent to the C-STORE SCP.

Centricity Radiology RA 600 is able to send data formerly received or stored in JPEG Lossy format in any uncompressed or JPEG Lossless format, or in the original JPEG Lossy format, but it will not decompress the pixel data and subsequently recompress it in a (different) lossy compression format.

When storing decompressed image data that was formerly stored in JPEG lossy format, the "Derivation Description" tag (0008,2111) and "Lossy Compression" tag (0008, 2112) will still specify that lossy JPEG compression had previously been applied to the pixel data and should still be shown to the user when the images are viewed. For more information see '3.1.3.2 Receive Images from a Remote System'.

3.1.2.2 Query a Remote Database

3.1.2.2.1 Associated Real World Activity

The user of the Centricity Radiology RA 600 system wants to have a view on a remote DICOM database and either views the complete contents of the remote database or fills out a query dialog box with fields for Patient Name, Patient ID, Study date, etc. Wildcards can be used instead of fully specified information to allow flexible queries. The contents of this dialog box and the requested columns in the Remote view can be fully configured, hence the contents of the Query data is dependent on the configuration.

3.1.2.2.2 Proposed Presentation Contexts

| Presentation Context Table for Remote Database Query | | | | | |
|------------------------------------------------------|-----------------------------|-------------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Patient Root Query/ Retrieve Model - FIND | 1.2.840.10008.5.1.4.1.2.1.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |
| Study Root Query/ Retrieve Model - FIND | 1.2.840.10008.5.1.4.1.2.2.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |
| Patient/Study Only Query/ Retrieve Model - FIND | 1.2.840.10008.5.1.4.1.2.3.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.2.2.3 SOP Specific Conformance Statement for SOP Class Query

The following keys are by default³ supported for the Patient Root Query:

| Level | Description | Tag |
|----------|-------------------------------------------|-------------|
| Patient | Specific Character Set | (0008,0005) |
| Patient | Patient's Name | (0010,0010) |
| Patient | Patient ID | (0010,0020) |
| Patient | Patient's Birth Date | (0010,0030) |
| Patient | Patient's Sex | (0010,0040) |
| Patient | Other Patient IDs | (0010,1000) |
| Study | Specific Character Set | (0008,0005) |
| Study | Study Description | (0008,1030) |
| Study | Study Date | (0008,0020) |
| Study | Study Instance UID | (0020,000D) |
| Study | Study ID | (0020,0010) |
| Study | Performing Physician's Name | (0008,1050) |
| Study | Accession Number | (0008,0050) |
| Study | Number of Study Related Series | (0020,1206) |
| Study | Number of Study Related Instances/Images | (0020,1208) |
| Series | Series Instance UID | (0020,000E) |
| Series | Series number | (0020,0011) |
| Series | Modality | (0008,0060) |
| Series | Number of Series Related Instances/Images | (0020,1209) |
| Instance | Instance Number | (0020,0013) |
| Instance | Rows | (0028,0010) |
| Instance | Columns | (0028,0011) |

The Patient/Study levels in the table above are also supported for the Patient/Study Only Query. For a Study Root Query by default³ the following keys are supported:

| Level | Description | Tag |
|----------|-------------------------------------------|-------------|
| Study | Specific Character Set | (0008,0005) |
| Study | Patient's Name | (0010,0010) |
| Study | Patient ID | (0010,0020) |
| Study | Patient's Birth Date | (0010,0030) |
| Study | Patient's Sex | (0010,0040) |
| Study | Study Description | (0008,1030) |
| Study | Study Date | (0008,0020) |
| Study | Study Instance UID | (0020,000D) |
| Study | Study ID | (0020,0010) |
| Study | Performing Physician's Name | (0008,1050) |
| Study | Accession Number | (0008,0050) |
| Study | Number of Study Related Series | (0020,1206) |
| Study | Number of Study Related Instances/Images | (0020,1208) |
| Series | Series Instance UID | (0020,000E) |
| Series | Series number | (0020,0011) |
| Series | Modality | (0008,0060) |
| Series | Number of Series Related Instances/Images | (0020,1209) |
| Instance | Instance Number | (0020,0013) |
| Instance | Rows | (0028,0010) |
| Instance | Columns | (0028,0011) |

³ The user is able to add any valid DICOM tag to this query.

Centricity Radiology RA 600 expects the remote Query SCP to perform all of the following matching methods:

| Matching methods for Study/Patient Root Query | |
|-----------------------------------------------|--|
| Method | |
| Single Value Matching | |
| Universal Matching | |
| Wild Card Matching | |
| Range Matching | |

3.1.2.3 Retrieve from a Remote System

3.1.2.3.1 Associated Real World Activity

After a view on a remote DICOM database has been obtained the user makes a selection of one or more studies, series or images and subsequently presses the Import button. This will initiate the transfer of images from the remote system to the local database of Centricity Radiology RA 600.

Note that the Centricity Radiology RA 600 front-end application performs the C-MOVE operation while the destination of the resulting C-STORE operation is the Centricity Radiology RA 600 Connection Service.

3.1.2.3.2 Proposed Presentation Contexts

| Presentation Context Table for Remote System Retrieve | | | | | |
|-------------------------------------------------------|-----------------------------|-------------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Patient Root Query/ Retrieve Model - MOVE | 1.2.840.10008.5.1.4.1.2.1.2 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |
| Study Root Query/ Retrieve Model - MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |
| Patient/Study Only Query/ Retrieve Model - MOVE | 1.2.840.10008.5.1.4.1.2.3.2 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.2.3.3 SOP Specific Conformance Statement for SOP Class Retrieve

The Centricity Radiology RA 600 front-end application provides standard conformance.

3.1.2.4 Print to a remote Laser Imager

3.1.2.4.1 Associated Real World Activity

The Centricity Radiology RA 600 user selects a study in the local database and submits it to the Print Service as a job for the desired laser imager. The user can choose several parameters such as the layout of the film and number of copies.

Or:

The Centricity Radiology RA 600 user creates a Virtual Film Sheet print job from the studies available in the Viewing module and submits it as a job for the desired laser imager. On a per-image or per-sheet basis several parameters can be altered. When submitting the job the user can choose a few parameters, such as the number of copies.

3.1.2.4.2 Proposed Presentation Contexts

| Presentation Context Table for Remote System Retrieve | | | | | |
|--------------------------------------------------------------|------------------------|----------------------------|-------------------|-------------|-----------------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Basic Grayscale Print Management Meta | 1.2.840.10008.5.1.1.9 | Implicit VR, Little Endian | 1.2.840.10008.1.2 | SCU | None |
| Basic Color Print Management Meta | 1.2.840.10008.5.1.1.18 | Implicit VR, Little Endian | 1.2.840.10008.1.2 | SCU | None |
| Basic Annotation Box ⁴ | 1.2.840.10008.5.1.1.15 | Implicit VR, Little Endian | 1.2.840.10008.1.2 | SCU | None |
| Print Job | 1.2.840.10008.5.1.1.14 | Implicit VR, Little Endian | 1.2.840.10008.1.2 | SCU | None |

3.1.2.4.3 SOP Specific Conformance Statement for Meta SOP Classes Basic Grayscale and Color Print Management

The Centricity Radiology RA 600 Print Service supports the following mandatory SOP classes as defined by the Basic Grayscale Print Management Meta class:

| Supported SOP classes as Basic Grayscale Print Management Meta SOP class | |
|---------------------------------------------------------------------------------|------------------------|
| SOP Class Name | SOP Class UID |
| Basic Film Session | 1.2.840.10008.5.1.1.1 |
| Basic Film Box | 1.2.840.10008.5.1.1.2 |
| Basic Grayscale Image Box | 1.2.840.10008.5.1.1.4 |
| Printer | 1.2.840.10008.5.1.1.16 |

For the Basic Color Print Management Meta SOP class it supports:

| Supported SOP classes as Basic Color Print Management Meta SOP class | |
|-----------------------------------------------------------------------------|-------------------------|
| SOP Class Name | SOP Class UID |
| Basic Film Session | 1.2.840.10008.5.1.1.1 |
| Basic Film Box | 1.2.840.10008.5.1.1.2 |
| Basic Color Image Box | 1.2.840.10008.5.1.1.4.1 |
| Printer | 1.2.840.10008.5.1.1.16 |

⁴ The Basic Annotation Box SOP class is negotiated only if the Print Destination is configured for it

The Centricity Radiology RA 600 Print Service is able to send the appropriate data to printers that support True Size printing, both for grayscale printers and color printers. The Centricity Radiology RA 600 Print Service will send the pixel data in its native size and additionally sends the Requested Image Size (2020,0030), which is considered to be a request to the Print SCP to Print at that size.

Please note that there is no formal way in DICOM to verify whether a DICOM Print SCP actually supports True Size printing, and that some Print SCPs do not report a failure when the Requested Image Size (tag 2020,0030) was requested by the SCU but not supported by the SCP.

As a result Centricity Radiology RA 600 Print Service can be configured in a way that it seems that images will be printed True Size, while they are just printed at a different size. It is up to the system integrator to verify from the printer's DICOM Conformance Statement whether that printer supports True Size printing, before setting the True Size option in the configuration for that particular printer.

3.1.2.4.3.1 Conformance for SOP Class Basic Film Session

The Centricity Radiology RA 600 Print Service includes the following attributes in the N-CREATE for the Basic Film Session SOP class:

| Attributes for Basic Film Session SOP class N-CREATE | | |
|------------------------------------------------------|-------------|-----------------------------------------------------------------------------------|
| Description | Tag | Range of values |
| Number of Copies | (2000,0010) | 1-10000 (Max. user value configurable, default 5) |
| Print Priority | (2000,0020) | "LOW", "MED", "HIGH" (according to print priority in Centricity Radiology RA 600) |
| Medium Type | (2000,0030) | <configurable> |
| Film Destination | (2000,0040) | "MAGAZINE", "PROCESSOR", <more configurable> |
| Film Session Label | (2000,0050) | <configurable> |

The N-SET and N-ACTION are currently unused. The N-DELETE is used to delete the complete Basic Film Session SOP instance hierarchy.

3.1.2.4.3.2 Conformance for SOP Class Basic Film Box

The Centricity Radiology RA 600 Print Service includes the following attributes in the N-CREATE for the Basic Film Box SOP class:

| Attributes for Basic Film Box SOP class N-CREATE | | | |
|--------------------------------------------------|-------------|----------------|-----------------------------------------------------|
| Description | Tag | Usage | Range of values |
| Annotation Display Format (BAB) | (2010,0010) | A ⁵ | <configurable> ⁶ |
| Film Orientation | (2010,0040) | A | "PORTRAIT", "LANDSCAPE" |
| Film Size ID | (2010,0050) | A | <configurable> |
| Magnification Type | (2010,0060) | C ⁷ | "BILINEAR", "CUBIC", "NONE", <more configurable> |
| Max Density | (2010,0130) | C | <configurable> |
| Configuration Information | (2010,0150) | C | <configurable> |
| Smoothing Type | (2010,0080) | C | <configurable> |
| Border Density | (2010,0100) | C | <configurable> |
| Empty Image Density | (2010,0110) | C | <configurable> |
| Min Density | (2010,0120) | C | <configurable> |
| Trim | (2010,0140) | C ⁷ | "YES", "NO", "" |

The N-SET is currently unused. The N-ACTION is used to print a complete Basic Film Box SOP instance and N-DELETE is used to delete it after printing.

⁵ A means the attribute is always sent

⁶ This value determines the number of Basic Image Box positions

⁷ C means the attribute is only sent when not empty

3.1.2.4.3.3 Conformance for SOP Class Basic Grayscale Image Box

The Centricity Radiology RA 600 Print Service includes the following attributes in the N-SET for the Basic Grayscale Image SOP class:

| Attributes for Basic Grayscale Image SOP Box class N-SET | | | |
|----------------------------------------------------------|-------------|-----------------|-------------------------------|
| Description | Tag | Usage | Range of values |
| Image Position | (2020,0010) | A | 1... ⁸ |
| Preformatted Grayscale Image Sequence | (2020,0110) | A | |
| > Samples Per Pixel | (0028,0002) | A | 1 |
| > Photometric Interpretation | (0028,0004) | A | "MONOCHROME2" |
| > Rows | (0028,0010) | A | |
| > Columns | (0028,0011) | A | |
| > Pixel Aspect Ratio | (0028,0034) | A | |
| > Bits Allocated ⁹ | (0028,0100) | A | 8, 16 |
| > Bits Stored ¹ | (0028,0101) | A | 8, 12 |
| > High Bit ¹ | (0028,0102) | A | 7, 11 |
| > Pixel Representation | (0028,0103) | A | 0 |
| > Pixel Data | (7FE0,0010) | A | |
| Requested Image Size | (2020,0030) | C ¹⁰ | hor. size of the image in mm. |

3.1.2.4.3.4 Conformance for SOP Class Basic Color Image Box

The Centricity Radiology RA 600 Print Service includes the following attributes in the N-SET for the Basic Color Image Box SOP class:

| Attributes for Basic Color Image Box SOP class N-SET | | | |
|------------------------------------------------------|-------------|-----------------|-------------------------------|
| Description | Tag | Usage | Range of values |
| Image Position | (2020,0010) | A | 1... |
| Preformatted Color Image Sequence | (2020,0111) | A | |
| > Samples Per Pixel | (0028,0002) | A | 3 |
| > Photometric Interpretation | (0028,0004) | A | |
| > Planar Configuration | (0028,0006) | A | RGB |
| > Rows | (0028,0010) | A | |
| > Columns | (0028,0011) | A | |
| > Pixel Aspect Ratio | (0028,0034) | A | |
| > Bits Allocated | (0028,0100) | A | 8 |
| > Bits Stored | (0028,0101) | A | 8 |
| > High Bit | (0028,0102) | A | 7 |
| > Pixel Representation | (0028,0103) | A | 0 |
| > Pixel Data | (7FE0,0010) | A | |
| Requested Image Size | (2020,0030) | C ¹⁰ | hor. size of the image in mm. |

⁸ Depends on the chosen Image Display format

⁹ The Centricity Radiology RA 600 Print Service offers support for either 8 or 12-bit printing. For 12-bit printing Bits Allocated is set to 16, Bits Stored is set to 12, and High Bit is set to 11. For 8-bit printing the values are 8, 8, and 7 respectively.

¹⁰ Only sent when the 'true size' option is used, See additional note in section 3.1.2.4.3 on page 22

3.1.2.4.3.5 Conformance for SOP Class Printer

The Centricity Radiology RA 600 Print Service shall accept N-EVENT-REPORT and return confirmation accordingly.

Both the Centricity Radiology RA 600 front-end application (option DICOM Printer Status) and the Centricity Radiology RA 600 Print Service uses N-GET for the Printer SOP class to get information from the SCP.

3.1.2.4.4 SOP Specific Conformance for SOP Class Print Job

Centricity Radiology RA 600 can optionally request this SOP Class from the SCP. In case it is supported the Centricity Radiology RA 600 Print Service will track the progress of the current job via N-EVENT-REPORTs and will not send the next job before completion of the current job.

3.1.2.4.5 SOP Specific Conformance for SOP Class Basic Annotation Box

If the Print Destination is configured to use Basic Annotation Box, the Print Service will negotiate the SOP class when setting up the association. In case it is supported the Centricity Radiology RA 600 Print Service will send a Basic Annotation Box N-SET command after it creates the Basic Film Box, using the UID returned from the Basic Film Box N-CREATE.

| Attributes for Basic Annotation Box SOP class N-SET | | | |
|-----------------------------------------------------|-------------|-------|-----------------|
| Description | Tag | Usage | Range of values |
| Annotation Position | (2030,0010) | A | <configurable> |
| Text String | (2030,0020) | A | <configurable> |

3.1.2.4.6 Optional Meta SOP Classes for Basic Grayscale Print Management

Currently these are not supported by the Centricity Radiology RA 600 Print Service.

3.1.2.4.7 Optional Meta SOP Classes for Basic Color Print Management

Currently these are not supported by the Centricity Radiology RA 600 Print Service.

3.1.2.5 Retrieve a Modality Worklist from a Remote System

3.1.2.5.1 Associated Real World Activity

Centricity Radiology RA 600 can query for a Modality Worklist to aid in merging patient demographics into DICOM images. This prevents the need to enter patient demographics manually and consequently eliminates a source of typing errors.

3.1.2.5.2 Proposed Presentation Contexts

| Presentation Context Table for Modality Worklist Management | | | | | |
|-------------------------------------------------------------|------------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Modality Worklist Information Model – FIND | 1.2.840.10008.5.1.4.31 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.2.5.3 SOP Specific Conformance Statement for SOP Class Modality Worklist Management

Centricity Radiology RA 600 provides standard conformance.

The following keys are supported for the Modality Worklist Management:

| Supported keys for Modality Worklist Management | | | |
|-------------------------------------------------|---------------------------------------|-------------|------|
| Module | Description | Tag | Type |
| Scheduled Procedure Step | Scheduled Procedure Step Sequence | (0040,0100) | R |
| | >Scheduled Station AE Title | (0040,0001) | R |
| | >Scheduled Procedure Step Start Date | (0040,0002) | R |
| | >Scheduled Procedure Step Start Time | (0040,0003) | R |
| | >Modality | (0008,0060) | R |
| | >Scheduled Performing Physician | (0040,0006) | R |
| | >Scheduled Procedure Step Description | (0040,0007) | O |
| | >Scheduled Station Name | (0040,0010) | O |
| | >Scheduled Procedure Step Location | (0040,0011) | O |
| | >Pre-Medication | (0040,0012) | O |
| | >Scheduled Procedure Step ID | (0040,0009) | O |
| >Requested Contrast Agent | (0032,1070) | O | |
| Requested Procedure | Requested Procedure ID | (0040,1001) | O |
| | Requested Procedure Description | (0032,1060) | O |
| | Study Instance UID | (0020,000D) | O |
| | Requested Procedure Priority | (0040,1003) | O |
| | Patient Transport Arrangements | (0040,1004) | O |
| Imaging Service Request | Accession Number | (0008,0050) | O |
| | Requesting Physician | (0032,1032) | O |
| | Referring Physician's Name | (0008,0090) | O |
| | Study Status ID | (0032,000A) | O |
| | Study Priority ID | (0032,000C) | O |
| Visit Identification | Admission ID | (0038,0010) | O |
| Visit Status | Current Patient Location | (0038,0300) | O |
| Patient Identification | Patient's Name | (0010,0010) | R |
| | Patient ID | (0010,0020) | R |
| | Issuer of Patient ID | (0010,0021) | O |
| | Other Patient IDs | (0010,1000) | O |
| | Other Patient Names | (0010,1001) | O |

| Supported keys for Modality Worklist Management | | | |
|--------------------------------------------------------|--------------------------------|-------------|-------------|
| Module | Description | Tag | Type |
| | Patient's Birth Name | (0010,1005) | O |
| | Patient's Mother's Birth Name | (0010,1060) | O |
| | Medical Record Locator | (0010,1090) | O |
| Patient Demographic | Patient's Birth Date | (0010,0030) | O |
| | Patient's Birth Time | (0010,0032) | O |
| | Patient's Sex | (0010,0040) | O |
| | Patient's Size | (0010,1020) | O |
| | Patient's Weight | (0010,1030) | O |
| | Patient's Address | (0010,1040) | O |
| | Military Rank | (0010,1080) | O |
| | Branch of Service | (0010,1081) | O |
| | Country of Residence | (0010,2150) | O |
| | Region of Residence | (0010,2152) | O |
| | Patient's Telephone Numbers | (0010,2154) | O |
| | Ethnic Group | (0010,2160) | O |
| | Patient's Religious Preference | (0010,21F0) | O |
| | Patient Comments | (0010,4000) | O |
| Patient Medical | Medical Alerts | (0010,2000) | O |
| | Contrast Allergies | (0010,2110) | O |
| | Pregnancy Status | (0010,21C0) | O |
| | Special Needs | (0038,0050) | O |
| | Patient State | (0038,0500) | O |

Centricity Radiology RA 600 expects the remote Query SCP to perform all of the following Matching methods

| Matching methods for Study/Patient Root Query |
|------------------------------------------------------|
| Method |
| Single Value Matching |
| Universal Matching |
| Wild Card Matching |
| Range Matching |

Centricity Radiology RA 600 may fill no, one, or multiple attributes in the query request with a non-empty value. Centricity Radiology RA 600 may thus request matching on Optional Matching Key Attributes.

All fields listed above are always included in the query request to ask the SCP to return them for each response. Centricity Radiology RA 600 expects the SCP to return values for all 'R' attributes whereas the attributes marked with 'O' may be optionally filled. Therefore Centricity Radiology RA 600 treats these attributes as Type 3 Return Key Attributes.

3.1.2.6 Send Modality Performed Procedure Step Messages to a Remote System

3.1.2.6.1 Associated Real World Activity

Centricity Radiology RA 600 can send Modality Performed Procedure Step messages (N-CREATE, N-SET) to remote systems, in order to indicate the completion or the discontinuation of a worklist operation.

Centricity Radiology RA 600 Modality Performed Procedure Step (MPPS) functionality is embedded in the optional Quality Control Module. When configured properly, the MPPS N-CREATE command and the MPPS N-SET command are sent to the configurable AE, one immediately after the other.

MPPS Completion messages can be sent after the user performed a manual match between a study in the local database and an item in the Worklist. The content of both MPPS transactions is collected from the selected item in the DICOM Modality Worklist and the study involved. No user extra input is requested for this operation.

MPPS Discontinue messages can be sent after selecting one single item in the worklist control on the Quality Control Module's desktop (right mouse button menu). When sending a discontinue message, the content of both MPPS transactions is collected from the selected item in the DICOM Modality Worklist.

3.1.2.6.2 Proposed Presentation Contexts

| Presentation Context Table for Modality Worklist Management | | | | | |
|-------------------------------------------------------------|-------------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Modality Performed Procedure Step | 1.2.840.10008.3.1.2.3.3 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.2.6.3 SOP Specific Conformance Statement for SOP Class Modality Performed Procedure Step

Centricity Radiology RA 600 provides standard conformance.

The following keys are supported for the Modality Performed Procedure Step N-CREATE :

| Supported keys for Modality Performed Procedure Step N-CREATE | | | |
|---------------------------------------------------------------|-----------------------------------|-------------|-----------------|
| Module | Description | Tag | Type |
| Performed Procedure Step Relationship | Patient's Name | (0010,0010) | R ¹¹ |
| | Patient ID | (0010,0020) | R ¹¹ |
| | Patient's Birth Date | (0010,0030) | R ¹¹ |
| | Patient's Sex | (0010,0040) | R ¹¹ |
| | Referenced Patient Sequence | (0008,1120) | R ¹² |
| | >Referenced SOP Class UID | (0008,1150) | - |
| | >Referenced SOP Instance UID | (0008,1155) | - |
| | Scheduled Step Attribute Sequence | (0040,0270) | R |
| | >Study Instance UID | (0020,000D) | R ¹³ |
| | >Referenced Study Sequence | (0008,1110) | R ¹² |

¹¹ The information is copied from the study data involved

¹² Always sent empty

¹³ The Study Instance UID (0020,000D) is copied from the resulting study in case of a completion message, and it is copied from the DICOM Modality Worklist in case of a discontinue message.

| | | | |
|--------------------------------------|----------------------------------------------|-------------|-----------------|
| | >>Referenced SOP Class UID | (0008,1150) | - |
| | >>Referenced SOP Instance UID | (0008,1155) | - |
| | >Accession Number | (0008,0050) | R ¹¹ |
| | >Placer Order Number/Imaging Service Request | (0040,2006) | O ¹⁴ |
| | >Filler Order Number/Imaging Service Request | (0040,2007) | O ¹⁴ |
| | >Placer Order Number/Imaging Service Request | (0040,2016) | O ¹⁴ |
| | >Filler Order Number/Imaging Service Request | (0040,2017) | O ¹⁴ |
| | >Requested Procedure ID | (0040,1001) | R ¹⁴ |
| | >Requested Procedure Description | (0032,1060) | R ¹⁴ |
| | >Placer Order Number/Procedure | (0040,1006) | O ¹⁴ |
| | >Filler Order Number/Procedure | (0040,1007) | O ¹⁴ |
| | >Scheduled Procedure Step ID | (0040,0009) | R ¹⁴ |
| | >Scheduled Procedure Step Description | (0040,0007) | R ¹⁴ |
| | >Scheduled Action Item Code Sequence | (0040,0008) | R ¹⁴ |
| | >>Code Value | (0008,0100) | O ¹⁴ |
| | >>Coding Scheme designator | (0008,0102) | O ¹⁴ |
| | >>Code Meaning | (0008,0104) | O ¹⁴ |
| Performed Procedure Step Information | Performed Station AE Title | (0040,0241) | R |
| | Performed Station Name | (0040,0242) | R |
| | Performed Location | (0040,0243) | R ¹² |
| | Performed Procedure Step Start Date | (0040,0244) | O ¹¹ |
| | Performed Procedure Step Start Time | (0040,0245) | O ¹¹ |
| | Performed Procedure Step ID | (0040,0253) | R ¹⁵ |
| | Performed Procedure Step Status | (0040,0252) | R |
| | Performed Procedure Step Description | (0040,0254) | R ¹¹ |
| | Comments on the Performed Procedure Step | (0040,0280) | - |
| | Performed Procedure Type Description | (0040,0255) | R ¹² |
| | Procedure Code Sequence | (0008,1032) | R ¹⁴ |
| | >Code Value | (0008,0100) | R |
| | >Coding Scheme Designator | (0008,0102) | R |
| | >Code Meaning | (0008,0104) | R |
| | Modality | (0008,0060) | R ¹⁶ |
| | Study ID | (0020,0010) | R ¹⁷ |
| | Performed Procedure Step End Date | (0040,0250) | R ¹⁸ |
| | Performed Procedure Step End Time | (0040,0251) | R ¹⁸ |
| | Performed Procedure Step Status | (0040,0252) | R ¹⁸ |

¹⁴ The information is copied from the DICOM Modality Worklist entry involved

¹⁵ The Performed Procedure Step ID is either copied from the study involved (if it was there) or generated by Centricity Radiology RA 600, according to a configurable format.

¹⁶ The field Modality (0008,0060) is copied from the resulting study in case of a completion message, and it is copied from the DICOM Modality Worklist in case of a discontinue message

¹⁷ The information is copied from the Study data involved

¹⁸ Inserted empty, filled in N-SET

| | | | |
|----------------------------------------------|----------------------------------------------|-------------|-----------------|
| Performed Procedure Step Acquisition Results | Performed Action Item Sequence | (0040,0260) | R ¹⁹ |
| | >Code Value | (0008,0100) | - |
| | >Coding Scheme Designator | (0008,0102) | - |
| | >Code Meaning | (0008,0104) | - |
| | Performed Series Sequence | (0040,0340) | R ¹¹ |
| | >Performing Physician's Name | (0008,1050) | R ¹¹ |
| | >Operator's Name | (0008,1070) | R ¹¹ |
| | >Protocol Name | (0018,1030) | R ¹¹ |
| | >Series Instance UID | (0020,000E) | R ¹¹ |
| | >Series Description | (0008,103E) | R ¹¹ |
| | >Retrieve AE Title | (0008,0054) | R ²⁰ |
| | >Referenced Image Sequence | (0008,1140) | R ¹¹ |
| | >>Referenced SOP Class UID | (0008,1150) | R ¹¹ |
| | >>Referenced SOP Instance UID | (0008,1155) | R ¹¹ |
| | >Referenced Standalone SOP Instance Sequence | (0040,0220) | - |
| | >>Referenced SOP Class UID | (0008,1150) | - |
| | >>Referenced SOP Instance UID | (0008,1155) | - |
| | Anatomic Structure, Space or Region Sequence | (0008,2229) | - |
| | >Code Value | (0008,0100) | - |

¹⁹ Always inserted as an empty field

²⁰ The retrieve AE Title is set to the AE Title of this **Centricity Radiology RA 600** installation

| | | | |
|----------------------------------------------------------------------|---------------------------------|-------------|-----------------|
| Performed Procedure Step Radiation Dose | >Coding Scheme Designator | (0008,0102) | - |
| | >Code Meaning | (0008,0104) | - |
| | Total Time of Fluoroscopy | (0040,0300) | O ¹⁴ |
| | Total Number of Exposures | (0040,0301) | O ¹⁴ |
| | Distance Source to Detector SID | (0018,1110) | O ¹⁴ |
| | Distance Source to Entrance | (0040,0306) | O ¹⁴ |
| | Entrance Dose | (0040,0302) | O ¹⁴ |
| | Exposed Area | (0040,0303) | O ¹⁴ |
| | Image Area Dose Product | (0018,115E) | O ¹⁴ |
| | Comments on Radiation Dose | (0040,0310) | O ¹⁴ |
| Performed Procedure Step Billing and Material Management | All Attributes | | - |

| Supported keys for Modality Performed Procedure Step N-SET | | | |
|------------------------------------------------------------|-----------------------------------|-------------|------|
| Module | Description | Tag | Type |
| Performed Procedure Step Information | Performed Procedure Step End Date | (0040,0250) | R |
| | Performed Procedure Step End Time | (0040,0251) | R |
| | Performed Procedure Step Status | (0040,0252) | R |

3.1.2.7 Verify the Committed Storage of Images on a Remote System

3.1.2.7.1 Associated Real World Activity

When Centricity Radiology RA 600 completes a transmission of images it can optionally verify whether the images have not only been received but also been stored successfully (committed) at the other end.

3.1.2.7.2 Proposed Presentation Contexts

| Presentation Context Table for Storage Commitment Push Model | | | | | |
|--------------------------------------------------------------|----------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.2.7.3 SOP Specific Conformance Statement for SOP Class Storage Commitment Push Model

Centricity Radiology RA 600 provides standard conformance. After the images and the storage commitment request have been sent, Centricity Radiology RA 600 will immediately close the association and will not wait for a reply from the SCP. Instead the SCP must open a new association to Centricity Radiology RA 600 in order to transmit the response. Thus the N-EVENT-REPORT must occur on a different association than the N-ACTION operation.

3.1.2.7.3.1 Operations

Centricity Radiology RA 600 can request storage commitment for all SOP classes as listed in the table in section 3.1.2.2.2. Centricity Radiology RA 600 supports the Referenced Study Component Sequence Attribute by including the Study Instance UID (0020,000D) of the requested objects. When storage commitment is requested for multiple studies, multiple requests are made, each on a separate association.

The validity of the Transaction UID that is generated for the storage commitment request is based on the system configuration. By default an answer must be obtained from the SCP within a configurable number of hours (default: 6 hours). After this the Transaction UID is no longer valid.

Centricity Radiology RA 600 does not support the optional Storage Media File-Set ID & UID attributes.

3.1.2.7.3.2 Notifications

When Centricity Radiology RA 600 receives a success status the status of the job that requested the storage commitment is changed from “Sent, waiting for storage commitment” to “Sent, storage commitment succeeded” and the job is finished. When deletion of the previously transmitted images is requested as part of the job they will be deleted.

When Centricity Radiology RA 600 receives a failure status the status of the job that requested the storage commitment is changed from “Sent, waiting for storage commitment” to “Error”. The job remains in the send queue in an error state and the specific reason for the error can be seen in the Details dialog. When deletion of the previously transmitted images is requested as part of the job this will not be done.

3.1.2.8 Convey a Study Status Change to a Remote System

3.1.2.8.1 Associated Real World Activity

The Centricity Radiology RA 600 Connection Service sends out a notification (N-EVENT-REPORT) to remote DICOM system, indicating that the study status of that system has changed.

3.1.2.8.2 Accepted Presentation Contexts

| Presentation Context Table | | | | | |
|----------------------------|-------------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Detached Study Management | 1.2.840.10008.3.1.2.3.1 | Implicit VR, Little Endian | 1.2.840.10008.1.2 | SCU | None |
| | | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | | |

3.1.2.8.3 SOP Specific Conformance Statement for SOP Class Detached Study Management

The Centricity Radiology RA 600 Connection Service provides standard conformance.

3.1.2.9 Request a Study Status Change from a Remote System

3.1.2.9.1 Associated Real World Activity

The Centricity Radiology RA 600 Connection Service sends out a request to a remote DICOM system, requesting the change of the study status for a certain study, residing on the remote system.

It will use a DICOM N-SET command for this.

3.1.2.9.2 Accepted Presentation Contexts

| Presentation Context Table | | | | | |
|----------------------------|-------------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Detached Study Management | 1.2.840.10008.3.1.2.3.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCU | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.2.9.3 SOP Specific Conformance Statement for SOP Class Detached Study Management

The Centricity Radiology RA 600 Connection Service provides standard conformance.

3.1.3 Association Acceptance Policy

The Centricity Radiology RA 600 Connection Service accepts associations for the following activities:

- Verification of the DICOM communication between a remote system and Centricity Radiology RA 600.
- Transfer of images from a remote system to Centricity Radiology RA 600.
- Processing of a query from a remote system.
- Initiation of a transfer of images to a remote system when a retrieve request is received.
- Commit the storage of images on a Centricity Radiology RA 600 system.
- Receive a Study Status Change Request from a remote system
- Receive a Study Status Change Event from a remote system

Centricity Radiology RA 600 Connection Service can be configured in a way that it will reject association requests from unknown applications. Centricity Radiology RA 600 connection service will always reject associations who use the wrong value for the called AE Title

3.1.3.1 Verify Communication with a Remote System

3.1.3.1.1 Associated Real World Activity

The Centricity Radiology RA 600 Connection Service will respond to verification request made by remote systems.

3.1.3.1.2 Accepted Presentation Contexts

| Presentation Context Table | | | | | |
|----------------------------|-------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Verification | 1.2.840.10008.1.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCP | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.3.1.3 SOP Specific Conformance Statement for SOP Class Verification

The Centricity Radiology RA 600 Connection Service provides standard conformance.

3.1.3.1.4 Presentation Context Acceptance Criterion

There are no specific rules for acceptance and prioritization of presentation contexts and the Centricity Radiology RA 600 Connection Service will accept all presentation contexts that match those listed in the table shown above.

3.1.3.2 Receive Images from a Remote System

3.1.3.2.1 Associated Real World Activity

A remote system wants to send images to the Centricity Radiology RA 600 system via the Centricity Radiology RA 600 Connection Service. Once the transfer is completed the new images will automatically be included in the user's view of the local database of Centricity Radiology RA 600 and can be selected for display.

3.1.3.2.2 Accepted Presentation Contexts

| Presentation Context Table for Receive From Remote System | | | | |
|-----------------------------------------------------------|--------------------------------|----------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | Role | Extended Negotiation |
| Name | UID | | | |
| CR Image | 1.2.840.10008.5.1.4.1.1.1 | See UID list A below | SCP | None |
| DX Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.1 | See UID list A below | SCP | None |
| DX Image (Process)* | 1.2.840.10008.5.1.4.1.1.1.1.1 | See UID list A below | SCP | None |
| DX Mammography Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.2 | See UID list A below | SCP | None |
| DX Mammography Image (Process)* | 1.2.840.10008.5.1.4.1.1.1.2.1 | See UID list A below | SCP | None |
| DX Intra-oral Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.3 | See UID list A below | SCP | None |
| DX Intra-oral Image (Process)* | 1.2.840.10008.5.1.4.1.1.1.3.1 | See UID list A below | SCP | None |
| CT Image | 1.2.840.10008.5.1.4.1.1.2 | See UID list A below | SCP | None |
| US Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.3 | See UID list A below | SCP | None |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 | See UID list A below | SCP | None |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 | See UID list A below | SCP | None |
| NM Image (Retired) | 1.2.840.10008.5.1.4.1.1.5 | See UID list A below | SCP | None |
| US Image (Retired) | 1.2.840.10008.5.1.4.1.1.6 | See UID list A below | SCP | None |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 | See UID list A below | SCP | None |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 | See UID list A below | SCP | None |
| Multi-Frame Single Bit SC Image | 1.2.840.10008.5.1.4.1.1.7.1 | See UID list A below | SCP | None |
| Multi-Frame Grayscale Byte SC Image | 1.2.840.10008.5.1.4.1.1.7.2 | See UID list A below | SCP | None |
| Multi-Frame Grayscale Word SC Image | 1.2.840.10008.5.1.4.1.1.7.3 | See UID list A below | SCP | None |
| Multi-Frame True Color SC Image | 1.2.840.10008.5.1.4.1.1.7.4 | See UID list A below | SCP | None |
| Standalone Overlay* | 1.2.840.10008.5.1.4.1.1.8 | See UID list B below | SCP | None |
| Standalone Curve* | 1.2.840.10008.5.1.4.1.1.9 | See UID list B below | SCP | None |
| Standalone Modality LUT* | 1.2.840.10008.5.1.4.1.1.10 | See UID list B below | SCP | None |
| Standalone VOI LUT* | 1.2.840.10008.5.1.4.1.1.11 | See UID list B below | SCP | None |
| Grayscale Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.1 | See UID list B below | SCP | None |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | See UID list A below | SCP | None |
| XF Image | 1.2.840.10008.5.1.4.1.1.12.2 | See UID list A below | SCP | None |
| NM Image | 1.2.840.10008.5.1.4.1.1.20 | See UID list A below | SCP | None |
| VL Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.1 | See UID list A below | SCP | None |
| VL Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.2 | See UID list A below | SCP | None |
| VL Endoscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.1 | See UID list A below | SCP | None |
| VL Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.2 | See UID list A below | SCP | None |
| VL Slide-Coordinates Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.3 | See UID list A below | SCP | None |
| VL Photographic Image | 1.2.840.10008.5.1.4.1.1.77.1.4 | See UID list A below | SCP | None |
| Basic Text Structured Reports | 1.2.840.10008.5.1.4.1.1.88.11 | See UID list B below | SCP | None |
| Enhanced Structured Reports* | 1.2.840.10008.5.1.4.1.1.88.22 | See UID list B below | SCP | None |
| Comprehensive Structured Reports* | 1.2.840.10008.5.1.4.1.1.88.33 | See UID list B below | SCP | None |
| Key Object Selection | 1.2.840.10008.5.1.4.1.1.88.59 | See UID list B below | SCP | None |
| PET Image | 1.2.840.10008.5.1.4.1.1.128 | See UID list A below | SCP | None |
| Standalone PET Curve* | 1.2.840.10008.5.1.4.1.1.129 | See UID list B below | SCP | None |
| RT Image | 1.2.840.10008.5.1.4.1.1.481.1 | See UID list A below | SCP | None |
| RT Dose* | 1.2.840.10008.5.1.4.1.1.481.2 | See UID list B below | SCP | None |
| RT Structure Set* | 1.2.840.10008.5.1.4.1.1.481.3 | See UID list B below | SCP | None |
| RT Beams Treatment Record* | 1.2.840.10008.5.1.4.1.1.481.4 | See UID list B below | SCP | None |
| RT Plan* | 1.2.840.10008.5.1.4.1.1.481.5 | See UID list B below | SCP | None |
| RT Brachy Treatment Record* | 1.2.840.10008.5.1.4.1.1.481.6 | See UID list B below | SCP | None |
| RT Treatment Summary Record* | 1.2.840.10008.5.1.4.1.1.481.7 | See UID list B below | SCP | None |

UID List A:

| Transfer Syntaxes for Reception of Image type IODs From Remote System | |
|------------------------------------------------------------------------------|------------------------|
| Name | UID |
| Implicit VR, Little Endian | 1.2.840.10008.1.2 |
| Explicit VR, Little Endian | 1.2.840.10008.1.2.1 |
| Explicit VR, Big Endian | 1.2.840.10008.1.2.2 |
| Explicit VR, Lossy JPEG 8-Bit Image Compression | 1.2.840.10008.1.2.4.50 |
| Explicit VR, Lossy JPEG 12-Bit Image Compression | 1.2.840.10008.1.2.4.51 |
| Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction | 1.2.840.10008.1.2.4.70 |
| Explicit VR, RLE Lossless compression | 1.2.840.10008.1.2.5 |
| Explicit VR, AMI Wavelet Progressive Lossy Compression | 1.2.528.1.1001.4.1.1.2 |
| Explicit VR, AMI JPEG Lossy Compression 8-bit | 1.2.528.1.1001.4.2.1.1 |
| Explicit VR, AMI JPEG Lossy Compression 12-bit | 1.2.528.1.1001.4.2.1.2 |
| Explicit VR, AMI ZLIB Lossless Compression | 1.2.528.1.1001.4.4.1 |

UID List B:

| Transfer Syntaxes for Reception of non-image type IODs From Remote System | |
|----------------------------------------------------------------------------------|---------------------|
| Name | UID |
| Implicit VR, Little Endian | 1.2.840.10008.1.2 |
| Explicit VR, Little Endian | 1.2.840.10008.1.2.1 |
| Explicit VR, Big Endian | 1.2.840.10008.1.2.2 |

Note: Centricity Radiology RA 600 is able to receive a large number of IODs. However, Centricity Radiology RA 600 will not always apply the intended behavior, described in the DICOM 3.0 2000 standard, for all of the IODs. IODs marked with a * symbol can only be received, stored, queried for and retrieved, and their contents can be displayed in a generic way. See section 3.1 Centricity Radiology RA 600 DICOM services AE Specifications for a detailed description of the visualization capabilities.

3.1.3.2.3 SOP Specific Conformance Statement for SOP Class Storage

The Centricity Radiology RA 600 Connection Service conforms to the full (level 2) conformance of the Storage SOP class. All Type 1, Type 2 and Type 3 attributes will be retained. In addition private attributes will be stored and included when the image is sent out again.

Upon successful storage of images of a study or series it may automatically be transferred to another system. The Centricity Radiology RA 600 system can be configured such to automatically delete studies or series from its local database when certain criteria are met.

When an image is received that has a SOP Instance UID (0008,0018) that is already present in the Centricity Radiology RA 600 database the transfers itself will complete successfully but the existing image in the database will be kept and the newly received image will be discarded.

When receiving images they will by default be stored in the (compressed, big/little endian) form they arrived. Upon further transmission of lossy compressed images decompression could take place if the negotiation results in an uncompressed or lossless compressed transfer syntax. The receiving system will have to check the Lossy Compression attribute (0028,1210) in order to verify that there was decompression loss when this image was created.

Centricity Radiology RA 600 will display the contents of attribute "Derivation Description" (0008,2111) or a descriptive text indicating prior compression loss along with the images, to ensure that the user is aware of the fact that derived pixel data is shown.

There is an option to automatically decompress lossy JPEG compressed images upon receiving, which is only there for performance reasons. The attribute Lossy Compression will be set to "01" and never changed ever after. The attribute "Derivative Description" (0008,2111) keeps its original contents and should still be displayed while viewing the images in third party applications.

Centricity Radiology RA 600 offers support for key images, adhering Supplement 59 of the DICOM 3.0 standard. In addition it is able to treat legacy Key Image labels of Image IODs, added by prior versions of Centricity Radiology RA 600 (i.e. when an image contains the attribute "Image Type" (0008,0008) which includes "KEY_IMAGE" as one of the multiple values then Centricity Radiology RA 600 will treat it as a Key Image).

Centricity Radiology RA 600 is able to receive and send any type of (color) image, i.e. images will not be rejected based on the value of tag Photometric Interpretation (0028,0004). However, Centricity Radiology RA 600 will only be able to display images with Photometric interpretation "MONochrome1", "MONochrome2", "RGB", "PALETTE COLOR", "YBR_FULL" and "YBR_FULL_422". For RGB and YBR_FULL images both planar configuration 0 (Color By Plane) and 1 (Color by Pixel) can be displayed.

3.1.3.2.4 Presentation Context Acceptance Criterion

There are no specific rules for acceptance and prioritization of presentation contexts and the Centricity Radiology RA 600 Connection Service will accept all presentation contexts that match those listed in the table shown above. It will however limit a certain SCU to only one association at a time. This means that when a SCU tries to initiate a request while any previous associations that it made are not completely processed that association will be accepted but actual data transfer will be postponed until all previous associations are completed.

Centricity Radiology RA 600 will accept the first Transfer Syntax from the list it accepts. In case of problems there are configuration options to turn off the acceptance of one or more specific Transfer Syntaxes, in order to make Centricity Radiology RA 600 select a different Transfer Syntax.

3.1.3.3 Query the Centricity Radiology RA 600 Database

3.1.3.3.1 Associated Real World Activity

A remote system wants to see which studies are available on the Centricity Radiology RA 600 system and issues a query.

3.1.3.3.2 Accepted Presentation Contexts

| Presentation Context Table for local Database Query | | | | | |
|-----------------------------------------------------|-----------------------------|-------------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Patient Root Query/ Retrieve Model - FIND | 1.2.840.10008.5.1.4.1.2.1.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCP | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |
| Study Root Query/ Retrieve Model - FIND | 1.2.840.10008.5.1.4.1.2.2.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCP | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.3.3.3 SOP Specific Conformance Statement for SOP Class Query

The Centricity Radiology RA 600 Database Service does not support relational queries. The following keys are by default²¹ supported for the Patient Root Query/Retrieve:

| Level | Description | Tag |
|---------|------------------------------------------|-------------|
| PATIENT | Specific Character Set | (0008,0005) |
| PATIENT | Patient Name | (0010,0010) |
| PATIENT | Patient ID | (0010,0020) |
| PATIENT | Other Patient Ids | (0010,1000) |
| PATIENT | Patients Date of Birth | (0010,0030) |
| PATIENT | Patients Sex | (0010,0040) |
| STUDY | Specific Character Set | (0008,0005) |
| STUDY | Study Date | (0008,0020) |
| STUDY | Study Time | (0008,0030) |
| STUDY | Accession Number | (0008,0050) |
| STUDY | Modalities in Study | (0008,0061) |
| STUDY | Referring Physician | (0008,0090) |
| STUDY | Study Description | (0008,1030) |
| STUDY | Patient Name | (0010,0010) |
| STUDY | Patient ID | (0010,0020) |
| STUDY | Study UID | (0020,000D) |
| STUDY | Study ID | (0020,0010) |
| STUDY | Study Status ID | (0032,000A) |
| STUDY | Reading Physician | (0008,1060) |
| STUDY | Reason for Study | (0032,1030) |
| STUDY | Number of Study Related Series | (0020,1206) |
| STUDY | Number of Study Related Instances/Images | (0020,1208) |
| STUDY | Retrieve AE Title | (0008,0054) |
| STUDY | Instance availability | (0008,0056) |
| SERIES | Specific Character Set | (0008,0005) |
| SERIES | Modality | (0008,0060) |
| SERIES | Performing Physician | (0008,1050) |
| SERIES | Body Part | (0018,0015) |
| SERIES | Patient Position | (0018,5100) |
| SERIES | Series UID | (0020,000E) |
| SERIES | Series Number | (0020,0011) |

²¹ System integrators can configure Centricity Radiology RA 600 in a way that any DICOM tag (public/private) can be queried for, on any level.

| | | |
|--------|-------------------------------------------|-------------|
| SERIES | Laterality | (0020,0060) |
| SERIES | Series Date | (0008,0021) |
| SERIES | Series Time | (0008,0031) |
| SERIES | Description | (0008,103E) |
| SERIES | Protocol | (0018,1030) |
| SERIES | View Position | (0018,5101) |
| SERIES | Frame of Reference UID | (0020,0052) |
| SERIES | Smallest Pixel Value in Series | (0028,0108) |
| SERIES | Largest Pixel Value in Series | (0028,0109) |
| SERIES | Institution Name | (0008,0080) |
| SERIES | Station Name | (0008,1010) |
| SERIES | Number of Series Related Instances/Images | (0020,1209) |
| SERIES | Institutional Department Name | (0008,1040) |
| IMAGE | Repetition Time | (0018,0080) |
| IMAGE | Echo Time | (0018,0081) |
| IMAGE | Specific Character Set | (0008,0005) |
| IMAGE | SOP Class UID | (0008,0016) |
| IMAGE | SOP Instance UID | (0008,0018) |
| IMAGE | Image Number | (0020,0013) |
| IMAGE | Rows | (0028,0010) |
| IMAGE | Columns | (0028,0011) |
| IMAGE | Patient Orientation | (0020,0037) |
| IMAGE | Image Type | (0008,0008) |
| IMAGE | Derivation Description | (0008,2111) |
| IMAGE | Slice Thickness | (0018,0050) |
| IMAGE | Imager Pixel Spacing | (0018,1164) |
| IMAGE | Image Position (Patient) | (0020,0032) |
| IMAGE | Pixel Spacing | (0028,0030) |
| IMAGE | Pixel Aspect Ratio | (0028,0034) |
| IMAGE | Smallest Image Pixel Value | (0028,0106) |
| IMAGE | Largest Image Pixel Value | (0028,0107) |
| IMAGE | Window Center | (0028,1050) |
| IMAGE | Window Width | (0028,1051) |
| IMAGE | Window Center & Width Explanation | (0028,1055) |
| IMAGE | Lossy Image Compression | (0028,2110) |
| IMAGE | Rescale Intercept | (0028,1052) |
| IMAGE | Rescale Slope | (0028,1053) |
| IMAGE | Rescale Type | (0028,1054) |
| IMAGE | Contrast/Bolus Agent | (0018,0010) |
| IMAGE | Patient Orientation | (0020,0020) |
| IMAGE | Acquisition Number | (0020,0012) |
| IMAGE | Slice Location | (0020,1041) |
| IMAGE | Instance Creation Date | (0008,0012) |
| IMAGE | Instance Creation Time | (0008,0013) |
| IMAGE | Presentation Label | (0070,0080) |
| IMAGE | Presentation Description | (0070,0081) |
| IMAGE | Presentation Creation Date | (0070,0082) |
| IMAGE | Presentation Creation Time | (0070,0083) |
| IMAGE | Presentation Creator's Name | (0070,0084) |
| IMAGE | Completion Flag | (0040,A491) |
| IMAGE | Verification Flag | (0040,A493) |
| IMAGE | Content Date | (0008,0023) |
| IMAGE | Content Time | (0008,0033) |
| IMAGE | Verification Date/Time | (0040,A030) |

The following keys are by default²² supported for the Study Root Query/Retrieve:

| Level | Description | Tag |
|-------|------------------------|-------------|
| STUDY | Specific Character Set | (0008,0005) |
| STUDY | Patient Name | (0010,0010) |
| STUDY | Patient ID | (0010,0020) |
| STUDY | Other Patient Ids | (0010,1000) |
| STUDY | Patients Date of Birth | (0010,0030) |

²² System integrators can configure **Centricity Radiology RA 600** in a way that any DICOM tag (public/private) can be queried for, on any level.

| | | |
|--------|-------------------------------------------|-------------|
| STUDY | Patients Sex | (0010,0040) |
| STUDY | Study Date | (0008,0020) |
| STUDY | Study Time | (0008,0030) |
| STUDY | Accession Number | (0008,0050) |
| STUDY | Modalities in Study | (0008,0061) |
| STUDY | Referring Physician | (0008,0090) |
| STUDY | Study Description | (0008,1030) |
| STUDY | Patient Name | (0010,0010) |
| STUDY | Patient ID | (0010,0020) |
| STUDY | Study UID | (0020,000D) |
| STUDY | Study ID | (0020,0010) |
| STUDY | Study Status ID | (0032,000A) |
| STUDY | Reading Physician | (0008,1060) |
| STUDY | Reason for Study | (0032,1030) |
| STUDY | Number of Study Related Series | (0020,1206) |
| STUDY | Number of Study Related Instances/Images | (0020,1208) |
| STUDY | Retrieve AE Title | (0008,0054) |
| STUDY | Instance availability | (0008,0056) |
| SERIES | Specific Character Set | (0008,0005) |
| SERIES | Modality | (0008,0060) |
| SERIES | Performing Physician | (0008,1050) |
| SERIES | Body Part | (0018,0015) |
| SERIES | Patient Position | (0018,5100) |
| SERIES | Series UID | (0020,000E) |
| SERIES | Series Number | (0020,0011) |
| SERIES | Laterality | (0020,0060) |
| SERIES | Series Date | (0008,0021) |
| SERIES | Series Time | (0008,0031) |
| SERIES | Description | (0008,103E) |
| SERIES | Protocol | (0018,1030) |
| SERIES | View Position | (0018,5101) |
| SERIES | Frame of Reference UID | (0020,0052) |
| SERIES | Smallest Pixel Value in Series | (0028,0108) |
| SERIES | Largest Pixel Value in Series | (0028,0109) |
| SERIES | Institution Name | (0008,0080) |
| SERIES | Station Name | (0008,1010) |
| SERIES | Number of Series Related Instances/Images | (0020,1209) |
| SERIES | Institutional Department Name | (0008,1040) |
| SERIES | Number of Series Related Instances/Images | (0020,1209) |
| IMAGE | Repetition Time | (0018,0080) |
| IMAGE | Echo Time | (0018,0081) |
| IMAGE | Specific Character Set | (0008,0005) |
| IMAGE | SOP Class UID | (0008,0016) |
| IMAGE | SOP Instance UID | (0008,0018) |
| IMAGE | Image Number | (0020,0013) |
| IMAGE | Rows | (0028,0010) |
| IMAGE | Columns | (0028,0011) |
| IMAGE | Patient Orientation | (0020,0037) |
| IMAGE | Image Type | (0008,0008) |
| IMAGE | Derivation Description | (0008,2111) |
| IMAGE | Slice Thickness | (0018,0050) |
| IMAGE | Imager Pixel Spacing | (0018,1164) |
| IMAGE | Image Position (Patient) | (0020,0032) |
| IMAGE | Pixel Spacing | (0028,0030) |
| IMAGE | Pixel Aspect Ratio | (0028,0034) |
| IMAGE | Smallest Image Pixel Value | (0028,0106) |
| IMAGE | Largest Image Pixel Value | (0028,0107) |
| IMAGE | Window Center | (0028,1050) |
| IMAGE | Window Width | (0028,1051) |
| IMAGE | Window Center & Width Explanation | (0028,1055) |
| IMAGE | Lossy Image Compression | (0028,2110) |
| IMAGE | Rescale Intercept | (0028,1052) |
| IMAGE | Rescale Slope | (0028,1053) |
| IMAGE | Rescale Type | (0028,1054) |
| IMAGE | Contrast/Bolus Agent | (0018,0010) |
| IMAGE | Patient Orientation | (0020,0020) |
| IMAGE | Acquisition Number | (0020,0012) |
| IMAGE | Slice Location | (0020,1041) |
| IMAGE | Instance Creation Date | (0008,0012) |

| | | |
|-------|-----------------------------|-------------|
| IMAGE | Instance Creation Time | (0008,0013) |
| IMAGE | Presentation Label | (0070,0080) |
| IMAGE | Presentation Description | (0070,0081) |
| IMAGE | Presentation Creation Date | (0070,0082) |
| IMAGE | Presentation Creation Time | (0070,0083) |
| IMAGE | Presentation Creator's Name | (0070,0084) |
| IMAGE | Completion Flag | (0040,A491) |
| IMAGE | Verification Flag | (0040,A493) |
| IMAGE | Content Date | (0008,0023) |
| IMAGE | Content Time | (0008,0033) |
| IMAGE | Verification Date/Time | (0040,A030) |

The following types of attribute matching are supported:

| Matching methods for Study/Patient Root Query SCP | |
|----------------------------------------------------------|--|
| Method | |
| Single Value Matching | |
| Universal Matching | |
| Wild Card Matching | |
| Range Matching | |

3.1.3.3.4 Presentation Context Acceptance Criterion

There are no specific rules for acceptance and prioritization of presentation contexts and the Centricity Radiology RA 600 Connection Service will accept all presentation contexts that match those listed in the table shown above.

3.1.3.4 Retrieve from the Centricity Radiology RA 600 Database

3.1.3.4.1 Associated Real World Activity

A remote system wants to receive data available on the Centricity Radiology RA 600 system and issues a retrieve command.

3.1.3.4.2 Accepted Presentation Contexts

| Presentation Context Table for local Database Query | | | | | |
|-----------------------------------------------------|-----------------------------|-------------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Study Root Query/ Retrieve Model - MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCP | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.3.4.3 SOP Specific Conformance Statement for SOP Class Retrieve

The Centricity Radiology RA 600 Connection Service provides standard conformance.

In addition all images and other IODs of a study or series can be retrieved by providing a single Study Instance UID or a Study Instance UID with a Series Instance UID.

3.1.3.4.4 Presentation Context Acceptance Criterion

Centricity Radiology RA 600 Connection Service will only accept retrieve requests from DICOM systems for which it has been configured. There are no specific rules for acceptance and prioritization of presentation contexts.

3.1.3.5 Commit Storage of Images in the Centricity Radiology RA 600 Database

3.1.3.5.1 Associated Real World Activity

Centricity Radiology RA 600 can confirm the storage (availability) of images on the local system when it is asked to do so. Note however that Centricity Radiology RA 600 does not provide long term archiving and that therefore there is no guarantee that the committed images will remain on the system for a longer period of time (see also below).

3.1.3.5.2 Accepted Presentation Contexts

| Presentation Context Table for Storage Commitment Push Model | | | | | |
|--------------------------------------------------------------|----------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCP | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.3.5.3 SOP Specific Conformance Statement for SOP Class Storage Commitment Push Model

Centricity Radiology RA 600 provides standard conformance.

Centricity Radiology RA 600 will open a new association to the SCU for transmitting the response back and will not transmit the response using the association over which the storage commitment request was sent by the SCU (even if it is still open at the time of sending the response back). Thus the N-EVENT-REPORT will occur on a different association than the N-ACTION operation.

3.1.3.5.3.1 Operations

Centricity Radiology RA 600 only provides temporary commitment for the storage of images. This means that the system can be configured to auto delete studies based on priority rules. Centricity Radiology RA 600 offers a user interface to delete studies. Additionally Centricity Radiology RA 600 has a Delete Lock mechanism preventing studies to be auto-deleted or accidentally deleted by the user.

Centricity Radiology RA 600 should not be used as a long-term archive. If you want Centricity Radiology RA 600 to retain the received studies (e.g. send them to a long-term storage after Centricity Radiology RA 600 no longer needs it), it needs to be configured as such.

Centricity Radiology RA 600 supports the Referenced Study Component Sequence Attribute by treating it as a Study Instance UID (0020,000D), which is used to speed up the search for the requested objects. When no objects are found with this Study UID, or the Referenced Study Component Sequence Attribute was not present in the request, the complete database is searched for the requested objects.

Committed images can be retrieved via the normal Query/Retrieve mechanism.

3.1.3.5.3.2 Notifications

Upon receiving a storage commitment request Centricity Radiology RA 600 will first wait for a configurable interval (5 seconds by default). It will then verify up to configurable number of retries (3 by default), separated by a configurable interval (15 seconds by default), whether the requested objects are stored on the system. After a fully successful verification (all requested objects could be verified) it will send a N-EVENT-REPORT back to the requester on a dedicated association, reporting storage commitment. If after the last retry not all objects could be verified an N-EVENT-REPORT message is sent back with a list of committed objects and a list of uncommitted objects.

Centricity Radiology RA 600 does not support the optional Storage Media File-Set ID and UID attributes.

Centricity Radiology RA 600 does not support the optional Retrieve AE Title (0008,0054) for storage Commitment N-EVENT-REPORTs.

3.1.3.5.4 Presentation Context Acceptance Criterion

There are no specific rules for acceptance and prioritization of presentation contexts and Centricity Radiology RA 600 will accept all presentation contexts that match those listed in the table shown above.

3.1.3.6 Receive a Study Status Change Request from a remote system

3.1.3.6.1 Associated Real World Activity

3.1.3.6.2 Accepted Presentation Contexts

| Presentation Context Table for Detached Study Management | | | | | |
|----------------------------------------------------------|-------------------------|-------------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Detached Study Management | 1.2.840.10008.3.1.2.3.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCP | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.3.6.3 SOP Specific Conformance Statement for SOP Class Detached Study Management

Centricity Radiology RA 600 provides standard conformance.

3.1.3.6.3.1 Operations

Upon receiving an N-SET command containing the Study UID involved and the new Study Status ID for the study, the Centricity Radiology RA 600 Connection Service will request the study status change from the Centricity Radiology RA 600 Database Service. It will report an error if the study was not found.

3.1.3.6.4 Presentation Context Acceptance Criterion

There are no specific rules for acceptance and prioritization of presentation contexts and Centricity Radiology RA 600 will accept all presentation contexts that match those listed in the table shown above.

3.1.3.7 Receive a Study Status Change Event from a remote system

3.1.3.7.1 Associated Real World Activity

3.1.3.7.2 Accepted Presentation Contexts

| Presentation Context Table for Detached Study Management | | | | | |
|----------------------------------------------------------|-------------------------|----------------------------|---------------------|------|----------------------|
| Abstract Syntax | | Transfer Syntax | | Role | Extended Negotiation |
| Name | UID | Name | UID | | |
| Detached Study Management | 1.2.840.10008.3.1.2.3.1 | Explicit VR, Little Endian | 1.2.840.10008.1.2.1 | SCP | None |
| | | Implicit VR, Little Endian | 1.2.840.10008.1.2 | | |

3.1.3.7.3 SOP Specific Conformance Statement for SOP Class Detached Study Management.

Centricity Radiology RA 600 provides standard conformance.

3.1.3.7.3.1 Operations

Upon receiving an N-EVENT-REPORT command containing the Study UID involved and the new Study Status ID for the study, the Centricity Radiology RA 600 Connection Service will request the study status change from the Centricity Radiology RA 600 Database Service.

3.1.3.7.4 Presentation Context Acceptance Criterion


Centricity Radiology RA 600 Connection Service will only accept retrieve requests from DICOM systems for which it has been configured. There are no specific rules for acceptance and prioritization of presentation contexts.

3.2 Centricity Radiology RA 600 DICOM Media Server AE

Centricity Radiology RA 600 provides standard conformance to the DICOM Media Storage Service and File Format (PS 3.10) and the Media Storage Application Profiles (PS 3.11) as far as the reading of uncompressed and JPEG Lossless Non-Hierarchical First Order Prediction compressed images on CD-Recordable media is concerned.

3.2.1 Implementation Model

3.2.1.1 Application Data Flow Diagram

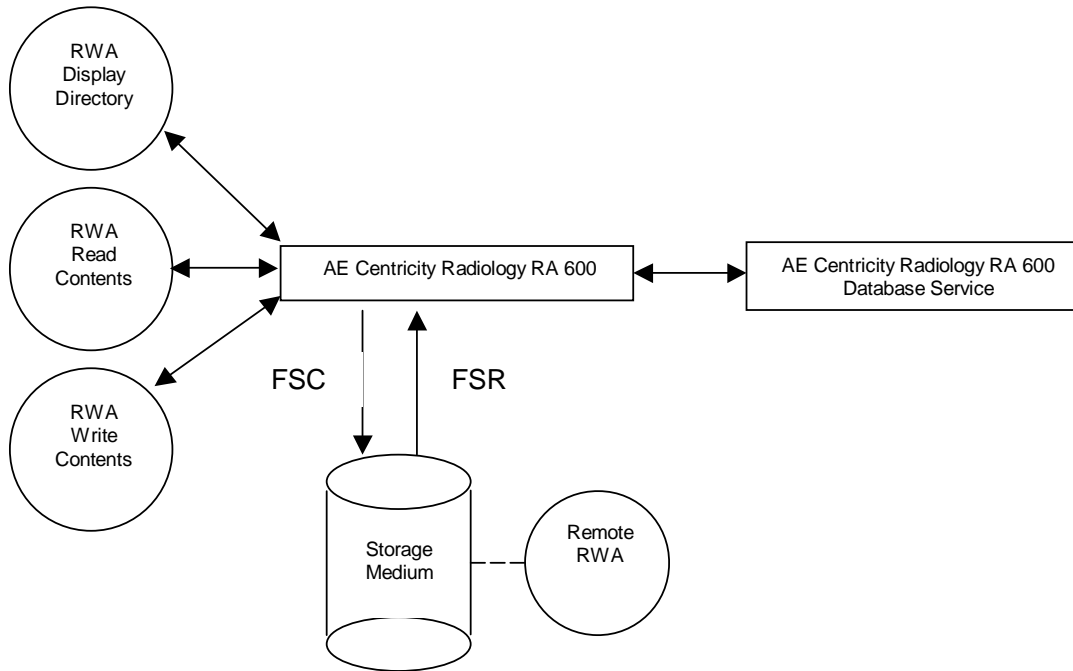

The Centricity Radiology RA 600 Media Server application flow consists of the following items:

- The Centricity Radiology RA 600 front-end application serves both as a FSC and a FSR. In this role it is able to read directory information from the storage medium, to import images from the storage medium and to write images and directory information to the storage medium.
- The three Real World Activities involved are available through the Centricity Radiology RA 600 AE's user interface.

Centricity Radiology RA 600 does not support writing of multi session CD-R disks.

3.2.1.2 File Meta Information Options

The Implementation Class UID is 1.2.528.1.1001.2.20020916.1

The Implementation Version Name is "AMI_DICOM01_2"

3.2.2 AE Specifications

3.2.2.1 Centricity Radiology RA 600 Application Entity Specification

Centricity Radiology RA 600 supports the following Standard Application Profiles, defined in DICOM 3.11 Annex A - E:

| Supported Application Profile | |
|--------------------------------------------------------|----------------------|
| Description | Identifier |
| General Purpose CD-R Image Interchange profile | STD-GEN-CD |
| General Purpose DVD-RAM Image Interchange profile | STD-GEN-DVD-RAM |
| Basic Cardiac X-Ray Angiographic Studies on CD-R Media | STD-XABC-CD |
| 1024 X-Ray Angiographic Studies on CD-R Media | STD-XA1K-CD |
| Image Display | STD-US-ID-SF-CDR |
| Image Display | STD-US-ID-SF-DVD-RAM |
| Image Display | STD-US-ID-MF-CDR |
| Image Display | STD-US-ID-MF-DVD-RAM |
| Spatial Calibration | STD-US-SC-SF-CDR |
| Spatial Calibration | STD-US-SC-SF-DVD-RAM |
| Spatial Calibration | STD-US-SC-MF-CDR |
| Spatial Calibration | STD-US-SC-MF-DVD-RAM |
| CT/MR Studies on CD-R | STD-CTMR-CD |
| CT/MR Studies on DVD-RAM | STD-CTMR-DVD-RAM |

In addition Centricity Radiology RA 600 supports the following application profiles, described in Annex A-C

| Supported Application Profile | |
|---------------------------------------------------------------|-------------------------------|
| Description | Identifier |
| GE Medical Systems Private Uncompressed – CDR | PRI-GEMS-UNCOMPRESSED-CDR |
| GE Medical Systems Private JPEG lossless compressed - CDR | PRI-GEMS-COMPRESSED-CDR |
| GE Medical Systems Private Uncompressed – DVD-RAM | PRI-GEMS-UNCOMPRESSED-DVD-RAM |
| GE Medical Systems Private JPEG lossless compressed – DVD-RAM | PRI-GEMS-COMPRESSED-DVD-RAM |
| GE Medical Systems Private CVIS Exchange – CDR | PRI-GEMS-CVIS-EXCHANGE |
| GE Medical Systems Private CVIS Archive – CDR | PRI-GEMS-CVIS-ARCHIVE |

3.2.2.2 Real-World Activities

Centricity Radiology RA 600 supports the following Real World Activities within the profile mentioned above:

| Real World Activities and roles ²³ | | | |
|-----------------------------------------------|--------------------------------|------|-------------|
| Supported Application Profiles | Real World Activity | Role | SC Option |
| STD-GEN-CD | Display Directory of CD-R disk | FSR | Interchange |
| STD-GEN-DVD-RAM | Read image(s) from CD-R disk | FSR | Interchange |
| STD-XABC-CD | Write image(s) on CD-R disk | FSC | Interchange |
| STD-XA1K-CD | | | |
| STD-US-ID-SF-CDR | | | |
| STD-US-ID-SF-DVD-RAM | | | |
| STD-US-ID-MF-CDR | | | |
| STD-US-ID-MF-DVD-RAM | | | |
| STD-US-SC-SF-CDR | | | |
| STD-US-SC-SF-DVD-RAM | | | |
| STD-US-SC-MF-CDR | | | |
| STD-US-SC-MF-DVD-RAM | | | |
| STD-US-CC-SF-CDR | | | |
| STD-US-CC-SF-DVD-RAM | | | |
| STD-US-CC-MF-CDR | | | |
| STD-US-CC-MF-DVD-RAM | | | |
| STD-CTMR-CD | | | |
| STD-CTMR-DVD-RAM | | | |
| PRI-GEMS-UNCOMPRESSED | | | |
| PRI-GEMS-COMPRESSED | | | |
| PRI-GEMS-CVIS-EXCHANGE | | | |
| PRI-GEMS-CVIS-ARCHIVE | | | |

3.2.2.2.1 Real World Activity: Display Directory of CD-R disk

Centricity Radiology RA 600 will act as a FSR when reading the directory of the medium. This will result in an overview of the patients, studies, series and images in Centricity Radiology RA 600 .

The display is structured in one of the following ways:

| Types of queries | |
|--------------------|-------------------------------|
| Type of query | Levels |
| Study Root Query | Study, Series, Image |
| Patient Root Query | Patient, Study, Series, Image |

At least the Patient Name and Patient ID fields are necessary for a correct display of the directory information. The following DICOMDIR keys are used for the user to be able to distinguish between the objects.

Reading of the directory contents is a standard feature of Centricity Radiology RA 600.

3.2.2.2.2 Real World Activity Read images from CD-R disk

Centricity Radiology RA 600 will act as a FSR when reading all/selected images from the CD-R medium. This feature will be available through the Import command or the View command from the Remote View area.

²³ The Centricity Radiology RA 600 software allows for more flexibility than this profile describes. Documentation for extended configuration is available.

Centricity Radiology RA 600 is able to read images/instances only if they belong to one of the following SOP classes:

| SOP classes for import of DICOM Part 10 images | |
|------------------------------------------------|--------------------------------|
| Name | UID |
| CR Image | 1.2.840.10008.5.1.4.1.1.1 |
| DX Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.1 |
| DX Image (Process)* | 1.2.840.10008.5.1.4.1.1.1.1.1 |
| DX Mammography Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.2 |
| DX Mammography Image (Process)* | 1.2.840.10008.5.1.4.1.1.1.2.1 |
| DX Intra-oral Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.3 |
| DX Intra-oral Image (Process)* | 1.2.840.10008.5.1.4.1.1.1.3.1 |
| CT Image | 1.2.840.10008.5.1.4.1.1.2 |
| US Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.3 |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 |
| NM Image (Retired) | 1.2.840.10008.5.1.4.1.1.5 |
| US Image (Retired) | 1.2.840.10008.5.1.4.1.1.6 |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 |
| Multi-Frame Single Bit SC Image | 1.2.840.10008.5.1.4.1.1.7.1 |
| Multi-Frame Grayscale Byte SC Image | 1.2.840.10008.5.1.4.1.1.7.2 |
| Multi-Frame Grayscale Word SC Image | 1.2.840.10008.5.1.4.1.1.7.3 |
| Multi-Frame True Color SC Image | 1.2.840.10008.5.1.4.1.1.7.4 |
| Standalone Overlay* | 1.2.840.10008.5.1.4.1.1.8 |
| Standalone Curve* | 1.2.840.10008.5.1.4.1.1.9 |
| Standalone Modality LUT* | 1.2.840.10008.5.1.4.1.1.10 |
| Standalone VOI LUT* | 1.2.840.10008.5.1.4.1.1.11 |
| Grayscale Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.1 |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 |
| XF Image | 1.2.840.10008.5.1.4.1.1.12.2 |
| NM Image | 1.2.840.10008.5.1.4.1.1.20 |
| VL Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.1 |
| VL Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.2 |
| VL Endoscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.1 |
| VL Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.2 |
| VL Slide-Coordinates Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.3 |
| VL Photographic Image | 1.2.840.10008.5.1.4.1.1.77.1.4 |
| Basic Text Structured Reports | 1.2.840.10008.5.1.4.1.1.88.11 |
| Enhanced Structured Reports | 1.2.840.10008.5.1.4.1.1.88.22 |
| Comprehensive Structured Reports* | 1.2.840.10008.5.1.4.1.1.88.33 |
| Key Object Selection | 1.2.840.10008.5.1.4.1.1.88.59 |
| PET Image | 1.2.840.10008.5.1.4.1.1.128 |
| Standalone PET Curve* | 1.2.840.10008.5.1.4.1.1.129 |
| RT Image | 1.2.840.10008.5.1.4.1.1.481.1 |
| RT Dose* | 1.2.840.10008.5.1.4.1.1.481.2 |
| RT Structure Set* | 1.2.840.10008.5.1.4.1.1.481.3 |
| RT Beams Treatment Record* | 1.2.840.10008.5.1.4.1.1.481.4 |
| RT Plan* | 1.2.840.10008.5.1.4.1.1.481.5 |
| RT Brachy Treatment Record* | 1.2.840.10008.5.1.4.1.1.481.6 |
| RT Treatment Summary Record* | 1.2.840.10008.5.1.4.1.1.481.7 |

IODs marked with a * symbol can be imported from CD-R into the local database, but their contents can only be displayed in a generic way. See section 3.1 Centricity Radiology RA 600 DICOM services AE Specifications for a detailed description of the visualization capabilities.

Centricity Radiology RA 600 is able to read images only if they have one of the following transfer syntaxes:

| Transfer syntaxes for import of DICOM Part 10 images | |
|----------------------------------------------------------------------|------------------------|
| Name | UID |
| Implicit VR, Little Endian | 1.2.840.10008.1.2 |
| Explicit VR, Little Endian | 1.2.840.10008.1.2.1 |
| Explicit VR, Big Endian | 1.2.840.10008.1.2.2 |
| Explicit VR, Lossy JPEG 8-Bit Image Compression | 1.2.840.10008.1.2.4.50 |
| Explicit VR, Lossy JPEG 12-Bit Image Compression | 1.2.840.10008.1.2.4.51 |
| Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction | 1.2.840.10008.1.2.4.70 |
| Explicit VR, RLE Lossless compression | 1.2.840.10008.1.2.5 |

Importing of studies from a DICOM Part 10 Volume is a standard feature of Centricity Radiology RA 600.

3.2.2.2.3 Real World Activity: Write images

Centricity Radiology RA 600 will act as a FSC when writing all or selected patients, studies or series from the local database view to random access archive media (like MODs). Centricity Radiology RA 600 uses a third party library from VOB Software GMBH to accomplish this.

Centricity Radiology RA 600 is able to write images of the following SOP classes:

| SOP classes for writing DICOM Part 10 images | |
|----------------------------------------------|--------------------------------|
| Name | UID |
| CR Image | 1.2.840.10008.5.1.4.1.1.1 |
| DX Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.1 |
| DX Image (Process) | 1.2.840.10008.5.1.4.1.1.1.1.1 |
| DX Mammography Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.2 |
| DX Mammography Image (Process) | 1.2.840.10008.5.1.4.1.1.1.2.1 |
| DX Intra-oral Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.3 |
| DX Intra-oral Image (Process) | 1.2.840.10008.5.1.4.1.1.1.3.1 |
| CT Image | 1.2.840.10008.5.1.4.1.1.2 |
| US Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.3 |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 |
| NM Image (Retired) | 1.2.840.10008.5.1.4.1.1.5 |
| US Image (Retired) | 1.2.840.10008.5.1.4.1.1.6 |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 |
| Multi-Frame Single Bit SC Image | 1.2.840.10008.5.1.4.1.1.7.1 |
| Multi-Frame Grayscale Byte SC Image | 1.2.840.10008.5.1.4.1.1.7.2 |
| Multi-Frame Grayscale Word SC Image | 1.2.840.10008.5.1.4.1.1.7.3 |
| Multi-Frame True Color SC Image | 1.2.840.10008.5.1.4.1.1.7.4 |
| Standalone Overlay | 1.2.840.10008.5.1.4.1.1.8 |
| Standalone Curve | 1.2.840.10008.5.1.4.1.1.9 |
| Standalone Modality LUT | 1.2.840.10008.5.1.4.1.1.10 |
| Standalone VOI LUT | 1.2.840.10008.5.1.4.1.1.11 |
| Grayscale Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.1 |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 |
| XF Image | 1.2.840.10008.5.1.4.1.1.12.2 |
| NM Image | 1.2.840.10008.5.1.4.1.1.20 |
| VL Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.1 |
| VL Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.2 |
| VL Endoscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.1 |
| VL Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.2 |
| VL Slide-Coordinates Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.3 |
| VL Photographic Image | 1.2.840.10008.5.1.4.1.1.77.1.4 |
| Basic Text Structured Reports | 1.2.840.10008.5.1.4.1.1.88.11 |
| Enhanced Structured Reports | 1.2.840.10008.5.1.4.1.1.88.22 |
| Comprehensive Structured Reports | 1.2.840.10008.5.1.4.1.1.88.33 |
| Key Object Selection | 1.2.840.10008.5.1.4.1.1.88.59 |
| PET Image | 1.2.840.10008.5.1.4.1.1.128 |
| Standalone PET Curve | 1.2.840.10008.5.1.4.1.1.129 |
| RT Image | 1.2.840.10008.5.1.4.1.1.481.1 |
| RT Dose | 1.2.840.10008.5.1.4.1.1.481.2 |
| RT Structure Set | 1.2.840.10008.5.1.4.1.1.481.3 |
| RT Beams Treatment Record | 1.2.840.10008.5.1.4.1.1.481.4 |
| RT Plan | 1.2.840.10008.5.1.4.1.1.481.5 |
| RT Brachy Treatment Record | 1.2.840.10008.5.1.4.1.1.481.6 |
| RT Treatment Summary Record | 1.2.840.10008.5.1.4.1.1.481.7 |

Writing studies to a DICOM Part 10 Volume is an optional feature of Centricity Radiology RA 600, which requires a separate license.

Centricity Radiology RA 600 creates DICOMDIR files for the DICOM Part 10 Volumes, containing the following keys:

| Keys exported to the DICOMDIR File | | | |
|------------------------------------|-----------------------------------|-------------|------|
| Directory Record Type | Key description | Tag | Type |
| PATIENT | Specific Character Set | (0008,0005) | 1C |
| PATIENT | Patient Name | (0010,0010) | 2 |
| PATIENT | Patient ID | (0010,0020) | 1 |
| PATIENT | Other Patient Ids | (0010,1000) | 3 |
| STUDY | Specific Character Set | (0008,0005) | 1C |
| STUDY | Study Date | (0008,0020) | 1 |
| STUDY | Study Time | (0008,0030) | 1 |
| STUDY | Accession Number | (0008,0050) | 2 |
| STUDY | Modalities in Study | (0008,0061) | 3 |
| STUDY | Referring Physician | (0008,0090) | 3 |
| STUDY | Study Description | (0008,1030) | 3 |
| STUDY | Patient Name | (0010,0010) | 2 |
| STUDY | Patient ID | (0010,0020) | 1 |
| STUDY | Patients Date of Birth | (0010,0030) | 2 |
| STUDY | Patients Sex | (0010,0040) | 2 |
| STUDY | Study UID | (0020,000D) | 1C |
| STUDY | Study ID | (0020,0010) | 1 |
| STUDY | Study Status ID | (0032,000A) | 3 |
| STUDY | Reading Physician | (0008,1060) | 3 |
| STUDY | Reason for Study | (0032,1030) | 3 |
| SERIES | Specific Character Set | (0008,0005) | 1C |
| SERIES | Modality | (0008,0060) | 1 |
| SERIES | Performing Physician | (0008,1050) | 3 |
| SERIES | Body Part | (0018,0015) | 3 |
| SERIES | Patient Position | (0018,5100) | 2C |
| SERIES | Series UID | (0020,000E) | 1 |
| SERIES | Series Number | (0020,0011) | 1 |
| SERIES | Laterality | (0020,0060) | 3 |
| SERIES | Series Date | (0008,0021) | 3 |
| SERIES | Series Time | (0008,0031) | 3 |
| SERIES | Description | (0008,103E) | 3 |
| SERIES | Protocol | (0018,1030) | 3 |
| SERIES | View Position | (0018,5101) | 2 |
| SERIES | Frame of Reference UID | (0020,0052) | 1 |
| SERIES | Smallest Pixel Value in Series | (0028,0108) | 3 |
| SERIES | Largest Pixel Value in Series | (0028,0109) | 3 |
| SERIES | Institution Name | (0008,0080) | 3 |
| SERIES | Station Name | (0008,1010) | 3 |
| SERIES | Institutional Department Name | (0008,1040) | 3 |
| IMAGE | Repetition Time | (0018,0080) | 2C |
| IMAGE | Echo Time | (0018,0081) | 2 |
| IMAGE | Specific Character Set | (0008,0005) | 1C |
| IMAGE | SOP Class UID | (0008,0016) | 1 |
| IMAGE | SOP Instance UID | (0008,0018) | 1C |
| IMAGE | Image Number | (0020,0013) | 1 |
| IMAGE | Rows | (0028,0010) | 3 |
| IMAGE | Columns | (0028,0011) | 3 |
| IMAGE | Patient Orientation | (0020,0037) | 2C |
| IMAGE | Image Type | (0008,0008) | 3 |
| IMAGE | Derivation Description | (0008,2111) | 3 |
| IMAGE | Slice Thickness | (0018,0050) | 2 |
| IMAGE | Imager Pixel Spacing | (0018,1164) | 3 |
| IMAGE | Image Position (Patient) | (0020,0032) | 2C |
| IMAGE | Pixel Spacing | (0028,0030) | 1 |
| IMAGE | Pixel Aspect Ratio | (0028,0034) | 1C |
| IMAGE | Smallest Image Pixel Value | (0028,0106) | 3 |
| IMAGE | Largest Image Pixel Value | (0028,0107) | 3 |
| IMAGE | Window Center | (0028,1050) | 1C |
| IMAGE | Window Width | (0028,1051) | 1C |
| IMAGE | Window Center & Width Explanation | (0028,1055) | 3 |
| IMAGE | Lossy Image Compression | (0028,2110) | 3 |
| IMAGE | Rescale Intercept | (0028,1052) | 1 |

| Keys exported to the DICOMDIR File | | | |
|------------------------------------|-----------------------------|-------------|------|
| Directory Record Type | Key description | Tag | Type |
| IMAGE | Rescale Slope | (0028,1053) | 1 |
| IMAGE | Rescale Type | (0028,1054) | 1 |
| IMAGE | Contrast/Bolus Agent | (0018,0010) | 2 |
| IMAGE | Patient Orientation | (0020,0020) | 2C |
| IMAGE | Acquisition Number | (0020,0012) | 3 |
| IMAGE | Slice Location | (0020,1041) | 3 |
| IMAGE | Instance Creation Date | (0008,0012) | 3 |
| IMAGE | Instance Creation Time | (0008,0013) | 3 |
| OVERLAY | Specific Character Set | (0008,0005) | 1C |
| OVERLAY | Overlay Number | (0020,0022) | 2 |
| MODALITY LUT | Specific Character Set | (0008,0005) | 1C |
| MODALITY LUT | Lookup table Number | (0020,0026) | 1 |
| VOI LUT | Specific Character Set | (0008,0005) | 1C |
| VOI LUT | Lookup table Number | (0020,0026) | 1 |
| CURVE | Specific Character Set | (0008,0005) | 1C |
| CURVE | Curve Number | (0020,0024) | 1 |
| PRESENTATION | Specific Character Set | (0008,0005) | 1C |
| PRESENTATION | SOP Instance UID | (0008,0018) | 1C |
| PRESENTATION | Instance Number | (0020,0013) | 1 |
| PRESENTATION | Presentation Label | (0070,0080) | 1 |
| PRESENTATION | Presentation Description | (0070,0081) | 2 |
| PRESENTATION | Presentation Creation Date | (0070,0082) | 1 |
| PRESENTATION | Presentation Creation Time | (0070,0083) | 1 |
| PRESENTATION | Presentation Creator's Name | (0070,0084) | 2 |
| PRESENTATION | Referenced Series Sequence | (0008,1115) | 1 |
| SR DOCUMENT | Instance Number | (0020,0013) | 1 |
| SR DOCUMENT | Completion Flag | (0040,A491) | 1 |
| SR DOCUMENT | Verification Flag | (0040,A493) | 1 |
| SR DOCUMENT | Content Date | (0008,0023) | 1 |
| SR DOCUMENT | Content Time | (0008,0033) | 1 |
| SR DOCUMENT | Verification Date/Time | (0040,A030) | 1C |
| SR DOCUMENT | Concept Name Code Sequence | (0040,A043) | 1 |
| SR DOCUMENT | Content Sequence | (0040,A730) | 1C |
| RT DOSE | Specific Character Set | (0008,0005) | 1C |
| RT DOSE | SOP Instance UID | (0008,0018) | 1C |
| RT DOSE | Instance Number | (0020,0013) | 1 |
| RT DOSE | Dose Summation Type | (3004,000A) | 1 |
| RT STRUCTURE SET | Specific Character Set | (0008,0005) | 1C |
| RT STRUCTURE SET | SOP Instance UID | (0008,0018) | 1C |
| RT STRUCTURE SET | Instance Number | (0020,0013) | 1 |
| RT STRUCTURE SET | Structure Set Label | (3006,0002) | 1 |
| RT STRUCTURE SET | Structure Set Date | (3006,0008) | 2 |
| RT STRUCTURE SET | Structure Set Time | (3006,0009) | 2 |
| RT PLAN | Specific Character Set | (0008,0005) | 1C |
| RT PLAN | SOP Instance UID | (0008,0018) | 1C |
| RT PLAN | Instance Number | (0020,0013) | 1 |
| RT PLAN | RT Plan Label | (300A,0002) | 1 |
| RT PLAN | RT Plan Date | (300A,0006) | 2 |
| RT PLAN | RT Plan Time | (300A,0007) | 2 |
| RT TREAT RECORD | Specific Character Set | (0008,0005) | 1C |
| RT TREAT RECORD | SOP Instance UID | (0008,0018) | 1C |
| RT TREAT RECORD | Instance Number | (0020,0013) | 1 |
| RT TREAT RECORD | Treatment Date | (3008,0250) | 2 |
| RT TREAT RECORD | Treatment Time | (3008,0251) | 2 |
| KEY OBJECT DOC | Instance Number | (0020,0013) | 1 |
| KEY OBJECT DOC | Content Date | (0008,0023) | 1 |
| KEY OBJECT DOC | Content Time | (0008,0033) | 1 |

3.2.3 Character Sets

Centricity Radiology RA 600 may change the value of the tag (0008,0005) Character Set on incoming studies before they are written to a DICOM Part 10 Medium. This will only happen if a user operation or automatic merge operation will change an existing IOD. This may lead to multi-valued Character Set values in cases where multiple non-ASCII scripts are used within the same IOD. In case the IODs contents haven't changed, the value for the Character Set (0008,0005) is retained and therefore depends on the system that created the DICOM IOD.

4 COMMUNICATION PROFILE

4.1 Supported Communication Stacks

The Centricity Radiology RA 600 DICOM services provide DICOM V3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

4.2 OSI Stack

Not supported.

4.3 TCP/IP Stack

The Centricity Radiology RA 600 DICOM services use the TCP/IP stack from the Microsoft Windows NT 4.0 or Microsoft Windows 2000 operating system on which it executes.

4.3.1 Physical Media Support

The Centricity Radiology RA 600 DICOM services are not dependent on the physical medium over which the TCP/IP executes.

4.4 Point-to-Point Stack

Not supported.

5 EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS

5.1 Standard Extended / Specialized / Private SOPs

5.1.1 GSPS objects referring to colour images

Centricity Radiology RA 600 is able to create Grayscale Softcopy Presentation State IODs containing references to color images. This mechanism is used to store measurements, annotations, and windowing operations and image transformations.

5.1.2 Collage IOD

Centricity Radiology RA 600 is able to create, send, receive and apply private IODs called Collages. Collages comprise a snapshot of the Front-end application, applicable when viewing images of one or more studies. A collage never copies information from images, Presentation states or key notes, but rather keeps references to these IODs, together with the position and display state. The collage IOD has been defined in terms of a basic structured report but has a separate SOP class UID as it serves a different goal.

5.1.2.1 SOP Class UID

Centricity Radiology RA 600 will use the following private SOP class UID to refer to a Collage IOD:

| UID Value | UID Name |
|------------------------|-------------------|
| 1.2.528.1.1001.5.1.1.1 | Collage (private) |

5.2 Private Transfer Syntaxes

Centricity Radiology RA 600 is able to use the following private transfer syntaxes for compressed exchange of image type IODs:

| Private Transfer Syntaxes for exchange of Image type IODs | |
|-----------------------------------------------------------|------------------------|
| Name | UID |
| Explicit VR, AMI Wavelet Progressive Lossy Compression | 1.2.528.1.1001.4.1.1.2 |
| Explicit VR, AMI JPEG Lossy Compression 8-bit | 1.2.528.1.1001.4.2.1.1 |
| Explicit VR, AMI JPEG Lossy Compression 12-bit | 1.2.528.1.1001.4.2.1.2 |
| Explicit VR, AMI ZLIB Lossless Compression | 1.2.528.1.1001.4.4.1 |

All Transfer Syntaxes listed above are based on the Explicit and Little Endian Transfer syntax, and use the encapsulated form of transferring Pixel Data in tag (7FE0,0010). The Value Representation for the Pixel Data tag will be OB.

5.3 Private Tags

5.3.1 Private tags created and used in GSPS objects

Private Creator Identification ("Applicare/RadWorks/Version 6.0")

| Attribute Name | Tag | VR | VM |
|----------------------------------|--------------|----|----|
| Annotation Type | (4105, XX01) | CS | 1 |
| Annotation Value | (4105, XX02) | DS | 1 |
| Cutline Image UID | (4105, XX03) | UI | 1 |
| Cutline Set UID | (4105, XX04) | UI | 1 |
| Annotation Color | (4105, XX05) | US | 1 |
| Annotation Line Style | (4105, XX06) | CS | 1 |
| Annotation Label | (4105, XX07) | SH | 1 |
| Annotation Creator | (4105, XX08) | PN | 1 |
| Annotation Creation Date | (4105, XX09) | DA | 1 |
| Annotation Creation Time | (4105, XX0A) | TM | 1 |
| Annotation Modification Sequence | (4105, XX0B) | SQ | 1 |
| Annotation Modifier | (4105, XX0C) | PN | 1 |
| Annotation Modification Date | (4105, XX0D) | DA | 1 |
| Annotation Modification Time | (4105, XX0E) | TM | 1 |
| Palette Color LUT Name | (4105, XX0F) | LO | 1 |
| Annotation Number | (4105, XX10) | US | 1 |

Private Creator Identification ("Applicare/RadWorks/Version 6.0")

| Attribute Name | Tag | VR | VM |
|------------------------------------|--------------|----|----|
| Requested Palette Color LUT (GSPS) | (4107, XX01) | SQ | 1 |

Private Creator Identification ("Applicare/RadWorks/Version 6.0/Summary")

| Attribute Name | Tag | VR | VM |
|----------------------------|--------------|----|----|
| Receive Origin Description | (3109, XX11) | ST | 1 |

5.3.2 Private tags, read from IODs

Private Creator Identification ("GE LUT Asymmetry Parameter")

| Attribute Name | Tag | VR | VM |
|----------------|--------------|----|----|
| LUT Asymmetry | (0045, XX67) | DS | 3 |

5.3.3 Private tags supported by the Query SCP (Study Level)

Private Creator Identification ("Applicare/RadWorks/Version 5.0")

| Attribute Name | Tag | VR | VM |
|----------------------------|--------------|----|----|
| Receive Origin Description | (3109, XX11) | ST | 1 |
| NEW/SEEN Status | (3109, XX02) | SH | 1 |
| Delete Lock | (3109, XX03) | CS | 1 |
| Receive Origin | (3109, XX08) | LO | 1 |
| Folder | (3109, XX09) | LO | 1 |
| Receive Date | (3109, XX0A) | DA | 1 |
| Receive Time | (3109, XX0B) | TM | 1 |
| Requested Compression | (3109, XX34) | CS | 1 |
| Study Lock | (3109, XX41) | CS | 1 |
| Archive Status | (3109, XX43) | CS | 1 |

6 CONFIGURATION

The configuration of the Centricity Radiology RA 600 DICOM services is stored in the Windows Registry. Only accounts (secured by passwords) with the right level of security will be able to change the configuration. This will typically be done by support personnel.

6.1 AE Title/Presentation Address Mapping

The AE title shared by the Centricity Radiology RA 600 services and front-end application is configurable and defaults to AE_<hostname>. The port on which the Centricity Radiology RA 600 Connection Service listens is also configurable and defaults to 104.

All remote systems that want to communicate with the Centricity Radiology RA 600 Connection Service have to be configured. For systems that want to act as SCUs of the Connection Service SCP SOP classes the following information may be needed:

- The AE title.
- The host name.
- The port number.

For systems with which the Centricity Radiology RA 600 DICOM services want to act as SCU the following information is needed:

- The AE title.
- The host name.
- The port number.

6.2 Configurable Parameters

Centricity Radiology RA 600 offers configuration of the following parameters, as far as the DICOM Communication is concerned.

| Configurable | | |
|-----------------------------|------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Name | Values | Description |
| Max. Number of Associations | 1... | Maximum number of simultaneous incoming associations accepted by the Connection Service |
| PDU Packet Size | 0 or 4096 – 4194304 | Proposed size of PDU packets, both in SCP and SCU role. The value of zero indicates that Centricity Radiology RA 600 is capable to accept PDU packets of any size. |
| Strict DICOM | True, False | Accept or reject incoming DICOM IODs when they contain type 1 violations. |
| Send Explicit VR | True, False | Determines whether or not Explicit Little Endian Transfer syntax is proposed when acting as a CStore SCU. |

7 SUPPORT OF EXTENDED CHARACTER SETS

Centricity Radiology RA 600 offers full support for the following character sets (possibly with code extension techniques):

| Supported Character Sets | |
|---------------------------------------|-----------------------------|
| Name | Value |
| Default Character repertoire ISO IR 6 | <none> |
| single-byte JIS X 0201 (Katakana) | ISO_IR 13, ISO 2022 IR 13 |
| single-byte JIS X 0201 (Romaji) | ISO_IR 14 |
| multi-byte JIS X 0208 (1983) | ISO 2022 IR 87 |
| Latin – 1 character repertoire | ISO_IR 100, ISO 2022 IR 100 |
| Latin – 2 character repertoire | ISO_IR 101, ISO 2022 IR 101 |
| Latin – 3 character repertoire | ISO_IR 109, ISO 2022 IR 109 |
| Latin – 4 character repertoire | ISO_IR 110, ISO 2022 IR 110 |
| Greek | ISO_IR 126, ISO 2022 IR 126 |
| Arabic | ISO_IR 127, ISO 2022 IR 127 |
| Hebrew | ISO_IR 138, ISO 2022 IR 138 |
| Cyrillic | ISO_IR 144, ISO 2022 IR 144 |
| Latin – 5 character repertoire | ISO_IR 148, ISO 2022 IR 148 |
| Multibyte KS X 1001 | ISO 2022 IR 149 |
| Multibyte JIS X 212 | ISO 2022 IR 159 |

In addition Centricity Radiology RA 600 offers support for the following universal character sets without code extensions:

| Supported Universal Character Sets | |
|------------------------------------|------------|
| Name | Value |
| Unicode in UTF-8 | ISO_IR 192 |
| GB18030 (GBK Chinese) | GB18030 |

Both character sets above have been described in Correction Proposal 252 of the DICOM 3.0 Standard, and are in Ballot phase as of the creation of this conformance statement. The support for reading DICOM data for any of these character sets is default behavior. Likewise, Centricity Radiology RA 600 will only write or send DICOM data using these character sets if the original data contained those. By default Centricity Radiology RA 600 is NOT able to create or modify data using these character sets.

Centricity Radiology RA 600 can be configured to create or modify data using either of the universal character sets described above. Please note that the use of these character sets is not yet common in the DICOM community and that this part of the standard has not yet been declared final. The use of these character sets can cause the inability to send DICOM data to other DICOM systems (including previous versions of Centricity Radiology RA 600) or DICOM Printers.

Annex A: GE Medical Systems Private Uncompressed Application Profile

A.1 CLASS AND PROFILE IDENTIFICATION

| Application Profile | Identifier | Description |
|-------------------------------------------------|-------------------------------|--------------------------------------------------------------------------------------------------------------------------------------|
| GE Medical Systems Private Uncompressed CDR | PRI-GEMS-UNCOMPRESSED-CDR | General purpose Explicit Little Endian for CDR, without icon-images and with limited DICOMDIR information on image level for CDR |
| GE Medical Systems Private Uncompressed DVD-RAM | PRI-GEMS-UNCOMPRESSED-DVD-RAM | General purpose Explicit Little Endian for CDR, without icon-images and with limited DICOMDIR information on image level for DVD-RAM |

A.2 CLINICAL CONTEXT

These profiles allow for generic storage purposes of IODS, with a minimum of DICOMDIR overhead.

A.2.1 ROLES AND SERVICE CLASS OPTIONS SECTION

The Application entity acting as a File-Set Creator generates a File Set under this Application Profile Class for purposes of archiving or exchange with other systems.

The role of File Set Reader shall be used by Application Entities that receive a transferred File Set, typically for review purposes.

The role of File Set Updater is undefined.

A.3 GENERAL CLASS PROFILE

A.3.1 SOP CLASSES AND TRANSFER SYNTAXES

| Information Object Definition | SOP Class UID | Transfer Syntax UID | FSC Req. | FSR Req. | FSU Req. |
|----------------------------------------|--------------------------------|---------------------------------------------------------------|----------|----------|----------|
| Basic Directory | 1.2.840.10008.1.3.10 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | Mand. | Mand. | Mand. |
| CR Image | 1.2.840.10008.5.1.4.1.1.1 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | Opt. | Opt. | Opt. |
| DX Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.1 | | | | |
| DX Image (Process) | 1.2.840.10008.5.1.4.1.1.1.1.1 | | | | |
| DX Mammography Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.2 | | | | |
| DX Mammography Image (Process) | 1.2.840.10008.5.1.4.1.1.1.2.1 | | | | |
| DX Intra-oral Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.3 | | | | |
| DX Intra-oral Image (Process) | 1.2.840.10008.5.1.4.1.1.1.3.1 | | | | |
| CT Image | 1.2.840.10008.5.1.4.1.1.2 | | | | |
| US Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.3 | | | | |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 | | | | |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 | | | | |
| NM Image (Retired) | 1.2.840.10008.5.1.4.1.1.5 | | | | |
| US Image (Retired) | 1.2.840.10008.5.1.4.1.1.6 | | | | |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 | | | | |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 | | | | |
| Multi-Frame Single Bit SC Image | 1.2.840.10008.5.1.4.1.1.7.1 | | | | |
| Multi-Frame Grayscale Byte SC Image | 1.2.840.10008.5.1.4.1.1.7.2 | | | | |
| Multi-Frame Grayscale Word SC Image | 1.2.840.10008.5.1.4.1.1.7.3 | | | | |
| Multi-Frame True Color SC Image | 1.2.840.10008.5.1.4.1.1.7.4 | | | | |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | | | | |
| XF Image | 1.2.840.10008.5.1.4.1.1.12.2 | | | | |
| NM Image | 1.2.840.10008.5.1.4.1.1.20 | | | | |
| VL Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.1 | | | | |
| VL Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.2 | | | | |
| VL Endoscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.1 | | | | |
| VL Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.2 | | | | |
| VL Slide-Coordinates Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.3 | | | | |
| VL Photographic Image | 1.2.840.10008.5.1.4.1.1.77.1.4 | | | | |
| PET Image | 1.2.840.10008.5.1.4.1.1.128 | | | | |
| RT Image | 1.2.840.10008.5.1.4.1.1.481.1 | | | | |
| Standalone Overlay | 1.2.840.10008.5.1.4.1.1.8 | | | | |
| Standalone Curve | 1.2.840.10008.5.1.4.1.1.9 | | | | |
| Standalone Modality LUT | 1.2.840.10008.5.1.4.1.1.10 | | | | |
| Standalone VOI LUT | 1.2.840.10008.5.1.4.1.1.11 | | | | |
| Grayscale Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.1 | | | | |
| Basic Text Structured Reports | 1.2.840.10008.5.1.4.1.1.88.11 | | | | |
| Enhanced Structured Reports | 1.2.840.10008.5.1.4.1.1.88.22 | | | | |
| Comprehensive Structured Reports | 1.2.840.10008.5.1.4.1.1.88.33 | | | | |
| Key Object Selection | 1.2.840.10008.5.1.4.1.1.88.59 | | | | |
| Standalone PET Curve | 1.2.840.10008.5.1.4.1.1.129 | | | | |
| RT Dose | 1.2.840.10008.5.1.4.1.1.481.2 | | | | |
| RT Structure Set | 1.2.840.10008.5.1.4.1.1.481.3 | | | | |
| RT Beams Treatment Record | 1.2.840.10008.5.1.4.1.1.481.4 | | | | |
| RT Plan | 1.2.840.10008.5.1.4.1.1.481.5 | | | | |
| RT Brachy Treatment Record | 1.2.840.10008.5.1.4.1.1.481.6 | | | | |
| RT Treatment Summary Record | 1.2.840.10008.5.1.4.1.1.481.7 | | | | |
| Collage (private) | 1.2.528.1.1001.5.1.1.1 | | | | |

A.3.2 PHYSICAL MEDIA AND MEDIA FORMATS

The profiles from this class require either

- the 120mm CD-R ISO/IEC 9660 Media Format, as defined in PS3.12 Annex F, or
- the 120mm DVD-RAM physical media with the DVD-RAM UDF1.5 Media Format, as defined in PS3.12 Annex J

A.3.3 DIRECTORY INFORMATION IN DICOMDIR

The profile is restricted to the following types of Directory Records: PATIENT, STUDY, SERIES, IMAGE, OVERLAY, MODALITY LUT, VOI LUT, CURVE, PRESENTATION, SR DOCUMENT, COLLAGE, RT DOSE, RT STRUCTURE SET, RT PLAN, RT TREAT RECORD, KEY OBJECT DOC

The profile does not impose restrictions or additional keys.

Annex B: GE Medical Systems Private Compressed Application Profile

B.1 CLASS AND PROFILE IDENTIFICATION

| Application Profile | Identifier | Description |
|-----------------------------------------------|-----------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| GE Medical Systems Private Compressed CDR | PRI-GEMS-COMPRESSED-CDR | General purpose Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction for CDR, without icon-images and with limited DICOMDIR information on image level. |
| GE Medical Systems Private Compressed DVD-RAM | PRI-GEMS-COMPRESSED-DVD-RAM | General Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction for DVD-RAM, without icon-images and with limited DICOMDIR information on image level. |

B.2 CLINICAL CONTEXT

These profiles allow for generic storage purposes of IODS, with a minimum of DICOMDIR overhead.

B.2.1 ROLES AND SERVICE CLASS OPTIONS SECTION

The Application entity acting as a File-Set Creator generates a File Set under this Application Profile Class for purposes of archiving or exchange with other systems. The profile is especially useful for systems that do not verify adherence to a profile

The role of File Set Reader shall be used by Application Entities that receive a transferred File Set, typically for review purposes.

The role of File Set Updater is undefined.

B.3 GENERAL CLASS PROFILE

B.3.1 SOP CLASSES AND TRANSFER SYNTAXES

| Information Object Definition | SOP Class UID | Transfer Syntax UID | FSC Req. | FSR Req. | FSU Req. | | | | |
|----------------------------------------|--------------------------------|------------------------------------------------------------------------------------------------|----------|----------|----------|---------------------------------------------------------------|--|--|--|
| Basic Directory | 1.2.840.10008.1.3.10 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | Mand. | Mand. | Mand. | | | | |
| CR Image | 1.2.840.10008.5.1.4.1.1.1 | Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction 1.2.840.10008.1.2.4.70 | Opt. | Opt. | Opt. | | | | |
| DX Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.1 | | | | | | | | |
| DX Image (Process) | 1.2.840.10008.5.1.4.1.1.1.1.1 | | | | | | | | |
| DX Mammography Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.2 | | | | | | | | |
| DX Mammography Image (Process) | 1.2.840.10008.5.1.4.1.1.1.2.1 | | | | | | | | |
| DX Intra-oral Image (Presentation) | 1.2.840.10008.5.1.4.1.1.1.3 | | | | | | | | |
| DX Intra-oral Image (Process) | 1.2.840.10008.5.1.4.1.1.1.3.1 | | | | | | | | |
| CT Image | 1.2.840.10008.5.1.4.1.1.2 | | | | | | | | |
| US Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.3 | | | | | | | | |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 | | | | | | | | |
| MR Image | 1.2.840.10008.5.1.4.1.1.4 | | | | | | | | |
| NM Image (Retired) | 1.2.840.10008.5.1.4.1.1.5 | | | | | | | | |
| US Image (Retired) | 1.2.840.10008.5.1.4.1.1.6 | | | | | | | | |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 | | | | | | | | |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 | | | | | | | | |
| Multi-Frame Single Bit SC Image | 1.2.840.10008.5.1.4.1.1.7.1 | | | | | | | | |
| Multi-Frame Grayscale Byte SC Image | 1.2.840.10008.5.1.4.1.1.7.2 | | | | | | | | |
| Multi-Frame Grayscale Word SC Image | 1.2.840.10008.5.1.4.1.1.7.3 | | | | | | | | |
| Multi-Frame True Color SC Image | 1.2.840.10008.5.1.4.1.1.7.4 | | | | | | | | |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | | | | | | | | |
| XF Image | 1.2.840.10008.5.1.4.1.1.12.2 | | | | | | | | |
| NM Image | 1.2.840.10008.5.1.4.1.1.20 | | | | | | | | |
| VL Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.1 | | | | | | | | |
| VL Multi-frame Image (Retired) | 1.2.840.10008.5.1.4.1.1.77.2 | | | | | | | | |
| VL Endoscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.1 | | | | | | | | |
| VL Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.2 | | | | | | | | |
| VL Slide-Coordinates Microscopic Image | 1.2.840.10008.5.1.4.1.1.77.1.3 | | | | | | | | |
| VL Photographic Image | 1.2.840.10008.5.1.4.1.1.77.1.4 | | | | | | | | |
| PET Image | 1.2.840.10008.5.1.4.1.1.128 | | | | | | | | |
| RT Image | 1.2.840.10008.5.1.4.1.1.481.1 | | | | | | | | |
| Standalone Overlay | 1.2.840.10008.5.1.4.1.1.8 | | | | | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | | | |
| Standalone Curve | 1.2.840.10008.5.1.4.1.1.9 | | | | | | | | |
| Standalone Modality LUT | 1.2.840.10008.5.1.4.1.1.10 | | | | | | | | |
| Standalone VOI LUT | 1.2.840.10008.5.1.4.1.1.11 | | | | | | | | |
| Grayscale Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.1 | | | | | | | | |
| Basic Text Structured Reports | 1.2.840.10008.5.1.4.1.1.88.11 | | | | | | | | |
| Enhanced Structured Reports | 1.2.840.10008.5.1.4.1.1.88.22 | | | | | | | | |
| Comprehensive Structured Reports | 1.2.840.10008.5.1.4.1.1.88.33 | | | | | | | | |
| Key Object Selection | 1.2.840.10008.5.1.4.1.1.88.59 | | | | | | | | |
| Standalone PET Curve | 1.2.840.10008.5.1.4.1.1.129 | | | | | | | | |
| RT Dose | 1.2.840.10008.5.1.4.1.1.481.2 | | | | | | | | |
| RT Structure Set | 1.2.840.10008.5.1.4.1.1.481.3 | | | | | | | | |
| RT Beams Treatment Record | 1.2.840.10008.5.1.4.1.1.481.4 | | | | | | | | |
| RT Plan | 1.2.840.10008.5.1.4.1.1.481.5 | | | | | | | | |
| RT Brachy Treatment Record | 1.2.840.10008.5.1.4.1.1.481.6 | | | | | | | | |
| RT Treatment Summary Record | 1.2.840.10008.5.1.4.1.1.481.7 | | | | | | | | |
| Collage (private) | 1.2.528.1.1001.5.1.1.1 | | | | | | | | |

B.3.2 PHYSICAL MEDIA AND MEDIA FORMATS

The profiles from this class require either

- the 120mm CD-R ISO/IEC 9660 Media Format, as defined in PS3.12 Annex F, or
- the 120mm DVD-RAM physical media with the DVD-RAM UDF1.5 Media Format, as defined in PS3.12 Annex J.

B.3.3 DIRECTORY INFORMATION IN DICOMDIR

The profile is restricted to the following types of Directory Records: PATIENT, STUDY, SERIES, IMAGE, OVERLAY, MODALITY LUT, VOI LUT, CURVE, PRESENTATION, SR DOCUMENT, COLLAGE, RT DOSE, RT STRUCTURE SET, RT PLAN, RT TREAT RECORD, KEY OBJECT DOC

The profile does not impose restrictions for additional keys

Annex C: GE Medical Systems Private Cardiac Exchange Profile

C.1 CLASS AND PROFILE IDENTIFICATION

| Application Profile | Identifier | Description |
|-------------------------------------------------|------------------------|--------------------------------------------------|
| GE Medical Systems Private Cardiac Exchange CDR | PRI-GEMS-CVIS-EXCHANGE | Profile for exchange of Cardiac US and XA images |

C.2 CLINICAL CONTEXT

This profile allows for exchange with the GEMS CVIS (Cardio Vascular Information System) of Cardiac images, conforming to a combination of the public STD-XABC, STD-US-ID-SF and STD-US-ID-MF profiles.

C.2.1 ROLES AND SERVICE CLASS OPTIONS SECTION

The Application entity acting as a File-Set Creator generates a File Set under this Application Profile Class for purposes of exchange with a CVIS system.

The role of File Set Reader shall be used by the Application Entity of the type CVIS which receive a transferred File Set, typically for review purposes.

The role of File Set Updater is undefined.

C.3 GENERAL CLASS PROFILE

C.3.1 SOP CLASSES AND TRANSFER SYNTAXES

| Information Object Definition | SOP Class UID | Transfer Syntax UID | FSC Req. | FSR Req. | FSU Req. |
|-------------------------------|------------------------------|------------------------------------------------------------------------------------------------|----------|----------|----------|
| Basic Directory | 1.2.840.10008.1.3.10 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | Mand. | Mand. | Mand. |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | Opt. | Opt. | Opt. |
| | | Explicit VR, RLE Lossless compression, 1.2.840.10008.1.2.5 | | | |
| | | Explicit VR, Lossy JPEG 8-Bit Image Compression 1.2.840.10008.1.2.4.50 | | | |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | | | |
| | | Explicit VR, RLE Lossless compression, 1.2.840.10008.1.2.5 | | | |
| | | Explicit VR, Lossy JPEG 8-Bit Image Compression 1.2.840.10008.1.2.4.50 | | | |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction 1.2.840.10008.1.2.4.70 | | | |

C.3.2 PHYSICAL MEDIA AND MEDIA FORMATS

The profiles from this class require the 120mm CD-R ISO/IEC 9660 Media Format, as defined in PS3.12 Annex F.

C.3.3 DIRECTORY INFORMATION IN DICOMDIR

The profile is restricted to the following types of Directory Records: PATIENT, STUDY, SERIES, and IMAGE.

The following additional keys shall be available in the DICOM file:

| Information Object Definition | SOP Class UID | Directory Record Type | Keys |
|-------------------------------|------------------------------|-----------------------|----------------------------------------------------------------------------------------|
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 | IMAGE | (0088,0200) |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 | | |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | PATIENT | (0010,0030) (0010,0040) |
| | | SERIES | (0008,0080) (0008,0081) (0008,1050) |
| | | IMAGE | (0088,0200) (0008,0008) (0050,0004) (0008,1140) (0008,1150) (0008,1155) |

The DICOMDIR file shall contain Icon Images.

C.4 SPECIFIC APPLICATION PROFILES

C.4.1 PRI-GEMS-CVIS-EXCHANGE

The CVIS Exchange profile imposes the following restrictions on the IODs:

| Information Object Definition | SOP Class UID | Transfer Syntax | Restrictions |
|----------------------------------|------------------------------------------------------------|------------------------|------------------------------------------------------------------------------------------------------|
| US Multi-frame Image US Image | 1.2.840.10008.5.1.4.1.1.3.1 1.2.840.10008.5.1.4.1.1.6.1 | 1.2.840.10008.1.2.1 | (0028,0004) one of "MONOCHROME2", "RGB", "PALETTE COLOR", "YBR_FULL_422", "YBR_PARTIAL_422" |
| | | 1.2.840.10008.1.2.5 | (0028,0004) one of "MONOCHROME2", "RGB", "PALETTE COLOR", "YBR_FULL" |
| | | 1.2.840.10008.1.2.4.50 | (0028,0004) one of "YBR_FULL_422", "YBR_PARTIAL_422" |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | 1.2.840.10008.1.2.4.70 | (0008,0060) = "XA" (0028,0010) <= 512 (0028,0011) <= 512 (0028,0100) = 8 (0028,0101) = 8 |

Annex D: GE Medical Systems Private Cardiac Archive Profile

D.1 CLASS AND PROFILE IDENTIFICATION

| Application Profile | Identifier | Description |
|------------------------------------------------|-----------------------|---------------------------------------------------|
| GE Medical Systems Private Cardiac Archive CDR | PRI-GEMS-CVIS-ARCHIVE | Profile for archiving of Cardiac US and XA images |

D.2 CLINICAL CONTEXT

This profile enables the user to create an archive CD, to be stored in the CVIS system. It basically consists of a combination of the public STD-XA1K, STD-US-ID-SF and STD-US-ID-MF profiles.

D.2.1 ROLES AND SERVICE CLASS OPTIONS SECTION

The Application entity acting as a File-Set Creator generates a File Set under this Application Profile Class for purposes of archiving to the CVIS system.

The role of File Set Reader shall be used by the Application Entity of the type CVIS.

The role of File Set Updater is undefined.

D.3 GENERAL CLASS PROFILE

D.3.1 SOP CLASSES AND TRANSFER SYNTAXES

| Information Object Definition | SOP Class UID | Transfer Syntax UID | FSC Req. | FSR Req. | FSU Req. |
|-------------------------------|------------------------------|------------------------------------------------------------------------------------------------|----------|----------|----------|
| Basic Directory | 1.2.840.10008.1.3.10 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | Mand. | Mand. | Mand. |
| US Multi-frame Image | 1.2.840.10008.5.1.4.1.1.3.1 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | Opt. | Opt. | Opt. |
| | | Explicit VR, RLE Lossless compression, 1.2.840.10008.1.2.5 | | | |
| | | Explicit VR, Lossy JPEG 8-Bit Image Compression 1.2.840.10008.1.2.4.50 | | | |
| US Image | 1.2.840.10008.5.1.4.1.1.6.1 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | | | |
| | | Explicit VR, RLE Lossless compression, 1.2.840.10008.1.2.5 | | | |
| | | Explicit VR, Lossy JPEG 8-Bit Image Compression 1.2.840.10008.1.2.4.50 | | | |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | Explicit VR, JPEG Lossless, Non-Hierarchical, First-Order Prediction 1.2.840.10008.1.2.4.70 | | | |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 | Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1 | | | |
| Standalone Overlay | 1.2.840.10008.5.1.4.1.1.8 | | | | |
| Standalone Curve | 1.2.840.10008.5.1.4.1.1.9 | | | | |

D.3.2 PHYSICAL MEDIA AND MEDIA FORMATS

The profiles from this class require the 120mm CD-R ISO/IEC 9660 Media Format, as defined in PS3.12 Annex F.

D.3.3 DIRECTORY INFORMATION IN DICOMDIR

The profile is restricted to the following types of Directory Records: PATIENT, STUDY, SERIES, and IMAGE.

The following additional keys shall be available in the DICOM file:

| Information Object Definition | SOP Class UID | Directory Record Type | Keys |
|----------------------------------|------------------------------------------------------------|-----------------------|----------------------------------------------------------------------------------------|
| US Multi-frame Image US Image | 1.2.840.10008.5.1.4.1.1.3.1 1.2.840.10008.5.1.4.1.1.6.1 | IMAGE | (0088,0200) |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | PATIENT | (0010,0030) (0010,0040) |
| | | SERIES | (0008,0080) (0008,0081) (0008,1050) |
| | | IMAGE | (0088,0200) (0008,0008) (0050,0004) (0008,1140) (0008,1150) (0008,1155) |

The DICOMDIR file shall contain Icon Images.

D.4 SPECIFIC APPLICATION PROFILES

D.4.1 PRI-GEMS-CVIS-ARCHIVE

The CVIS Archive profile imposes the following restriction on the IOD:

| Information Object Definition | SOP Class UID | Transfer Syntax | Restrictions |
|----------------------------------|------------------------------------------------------------|------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------|
| US Multi-frame Image US Image | 1.2.840.10008.5.1.4.1.1.3.1 1.2.840.10008.5.1.4.1.1.6.1 | 1.2.840.10008.1.2.1 | (0028,0004) one of "MONOCHROME2", "RGB", "PALETTE COLOR", "YBR_FULL_422", "YBR_PARTIAL_422" |
| | | 1.2.840.10008.1.2.5 | (0028,0004) one of "MONOCHROME2", "RGB", "PALETTE COLOR", "YBR_FULL" |
| | | 1.2.840.10008.1.2.4.50 | (0028,0004) one of "YBR_FULL_422", "YBR_PARTIAL_422" |
| XA Image | 1.2.840.10008.5.1.4.1.1.12.1 | 1.2.840.10008.1.2.4.70 | (0008,0060)="XA" (0028,0010) <= 1024 (0028,0011) <= 1024 (0028,0101) one of 8, 10, 12 |
| SC Image | 1.2.840.10008.5.1.4.1.1.7 | 1.2.840.10008.1.2.1 | (0028,0010) <= 1024 (0028,0011) <= 1024 (0028,0002)=1 (0028,0004)="MONOCHROME2" (0028,0100)=8 (0028,0101)=8 (0028,0102)=7 (0028,0103)=0 |