




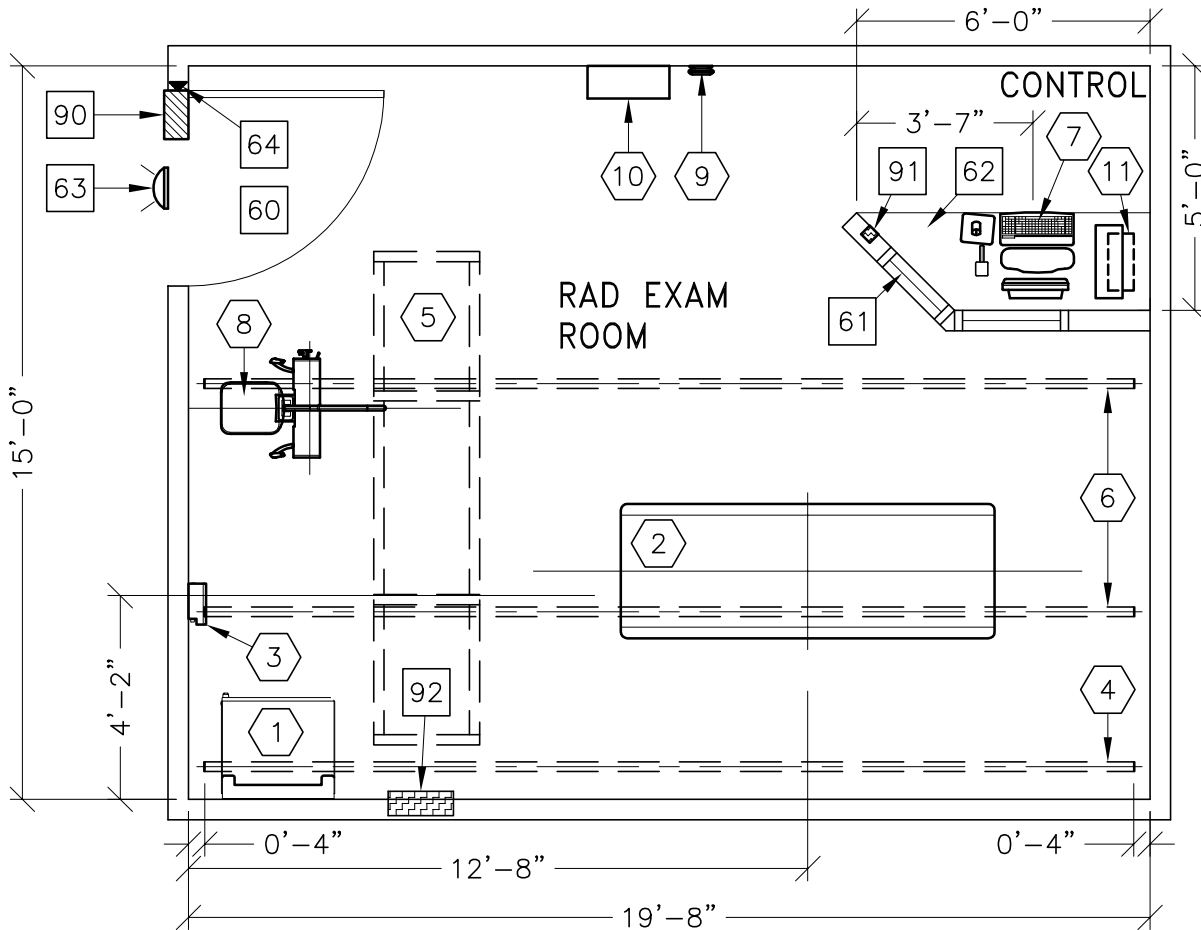

OPTIMA XR646 HD – STANDARD TABLE

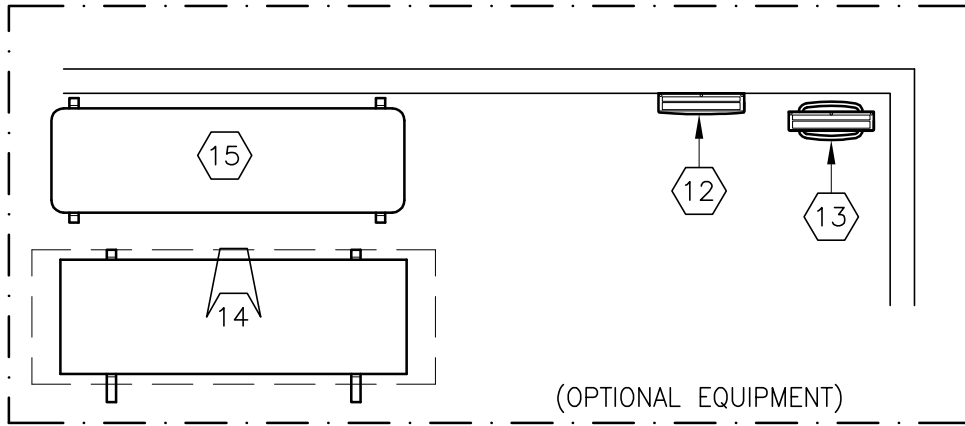

THE FOLLOWING SHOTS ARE NOT AVAILABLE IN THIS LAYOUT:
 REAR TO FRONT CROSS TABLE SHOT TO TABLE CENTERLINE



ROOM DIMENSIONS	LENGTH & WIDTH	CEILING HEIGHT
MINIMUM:	VARIABLES: BASED ON EQUIPMENT AND APPLICATIONS	8'-9 3/4" [2686mm]

ROOM PLAN LOCATED ON PAGE 1-164

ITEM	QUANTITY			
⬡	↓	ITEM DESCRIPTION	WEIGHT	HEAT OUTPUT
①	1	SYSTEM CABINET	705 lbs	2440 btu
②	1	STANDARD TABLE	705 lbs	372 btu
③	1	TETHER INTERFACE BOX	15 lbs	10 btu
④	1	CABLE DRAPE RAIL.	182 lbs	
⑤	1	XT RADIOGRAPHIC SUSPENSION WITH INBOARD MOUNTING.	764 lbs	105 btu
⑥	2	LONGITUDINAL STATIONARY RAIL FOR XT SUSPENSION	68 lbs	
⑦	1	OPERATORS CONSOLE	61 lbs	604 btu
⑧	1	MANUAL CHEST UNIT	573 lbs	136 btu
⑨	1	ACCESS POINT	2 lbs	
⑩	1	GRID HOLDER <FIELD VERIFY IDEAL LOCATION>	30 lbs	
— OPTIONAL —				
⑪	1	PARTIAL SYSTEM UNINTERRUPTIBLE POWER SUPPLY	77 lbs	30 btu
⑫	1	DETECTOR BIN <WALL MOUNT>	33 lbs	
⑬	1	DETECTOR BIN <FLOOR MOUNT>	33 lbs	
⑭	1	MOBILE TABLE	224 lbs	
⑮	1	CARBON FIBER TABLE	70 lbs	

ENVIRONMENT

Ambient Operation Temperature:	59-95° <F> [15-35° <C>]
Allowable Temperature Change:	<50° <F> [<10° <C>] per hour
Humidity:	30-60 percent non condensing
Allowable Humidity Change:	<30 percent per hour
Max - Altitude:	9,842.52 FT. [3000 M]

ROOM PLAN LOCATED ON PAGE 1-164

ITEM	QUANTITY	ITEM DESCRIPTION	WEIGHT	HEAT OUTPUT
<p>***** CUSTOMER/CONTRACTOR SUPPLIED AND INSTALLED ITEMS *****</p>				
60		<p>MINIMUM DOOR OPENING FOR EQUIPMENT DELIVERY IS 37.5 IN. W x 75 IN. H [950mm x 1900mm], CONTINGENT ON A 98.5 IN. [2500mm] CORRIDOR WIDTH NOTE: IMAGE PASTE OPTION REQUIRES AN 82 IN. H [2100mm] HIGH OPENING FOR ACCESS.</p>		
61		<p>CONTROL WALL, 7 FT. HIGH WITH LEAD GLASS VIEWING WINDOW.</p>		
62		<p>COUNTER TOP FOR EQUIPMENT- MINIMUM DEPTH 24 IN. AND ADDITIONAL SHELVING MAY BE REQUIRED BELOW COUNTER TOP FOR PC TOWER. PROVIDE GROMMETED OPENINGS AS REQUIRED TO ROUTE CABLES.</p>		
63		<p>X-RAY ON WARNING LIGHT - AVAILABLE FROM GE SUPPLY CALL: 800-200-9760 GE CAT. NO. WXIABWW-OF-XIU</p>		
64		<p>DOOR LIMIT SWITCH (NEEDED ONLY IF REQUIRED BY STATE/LOCAL CODES)</p>		
90		<p>X-RAY ROOM WARNING LIGHT CONTROL PANEL REFERENCE JUNCTION POINT 'XRLC' ON SHEET 'E1' FOR DETAILED DESCRIPTION -E4502RL FOR WARNING LIGHT CONTROL ONLY.</p>		
91		<p>EMERGENCY OFF SWITCH (NEEDED ONLY IF REQUIRED BY STATE/LOCAL CODES)</p>		
92		<p>MAIN DISCONNECT, REFERENCE JUNCTION POINT 'A' ON SHEET E1. (16" W x 24" H x 6" D)</p>		