


# Voluson SWIFT

Site  
Preparation

## Physical Dimensions and Weight (mm) :

Please Note: The picture may vary according to order configuration.

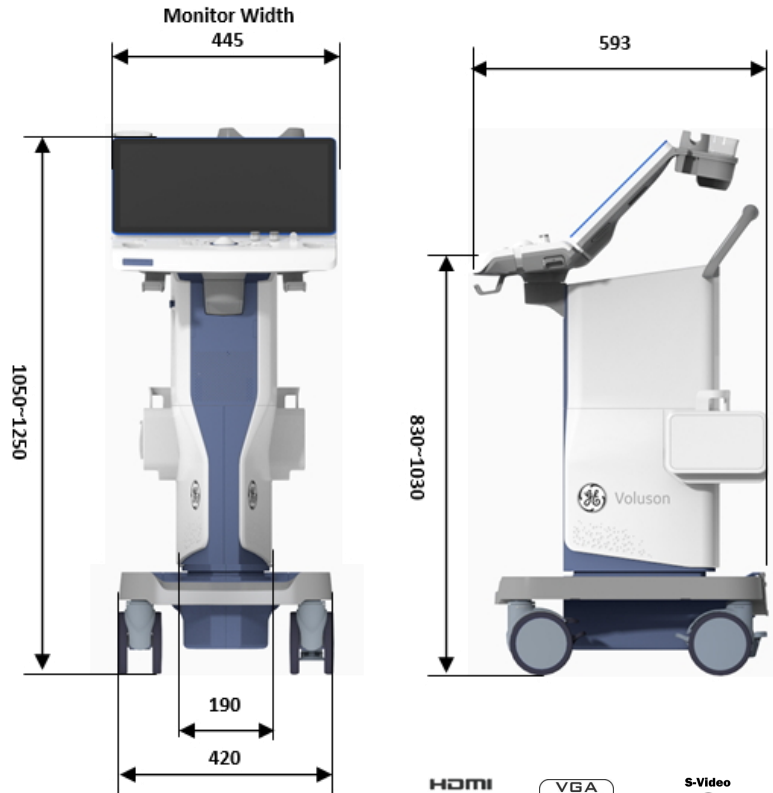

## External Inputs and Outputs :




## Environmental Requirements

Operating Temperature	18 to 30 C (64 to 86 F)
Operating Humidity	30 to 80% rH, non-condensing
Heat Dissipation	1200 BTU/hour +300 Btu for each person. Without on-board peripherals
Storage Temperature	-10 to 50 C (14 to 122 F)
Storage Humidity	10 to 90% rH, non-condensing
Lighting	Combination lighting system (dim/bright) is recommended. <b>Keep in mind that lighting controls and dimmers can be a source of EMI which could degrade image quality.</b>

Please Note: For more information please refer to the product's service & user manuals.

## Recommended Ultrasound Room Layout 4.3m x 5.2m (14ft x 17ft)

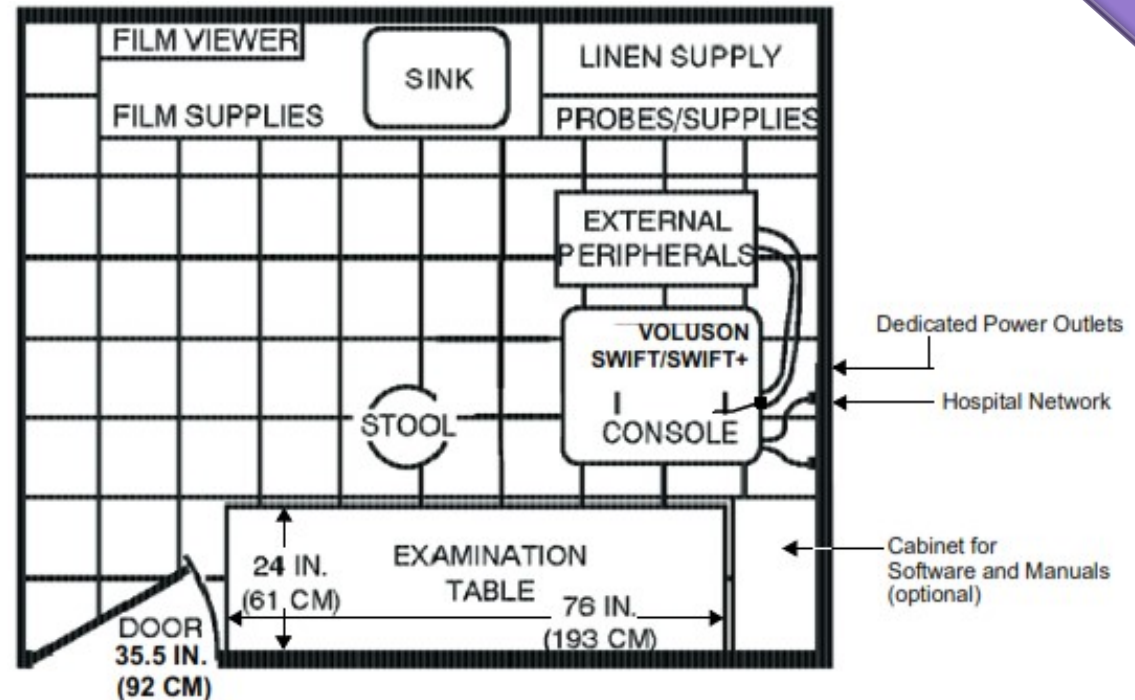

## Electrical Specifications

Voltage	100 - 240 VAC +-%10 / 4.5....1.8 A / 50, 60 Hz (2%)
Power Consumption	450 VA, including all on board peripherals.
Site Power Outlets	A dedicated AC power outlet must be within reach of the unit without extension cords
Power outage may occur	Requires a dedicated single branch circuit. To avoid circuit overload and possible loss of critical care equipment, make sure you DO NOT have any other equipment operating on the same circuit.
Acoustic Noise Output	max. 55 dB(A)