



***GE Medical Systems***

---

# **Technical Publications**

**Direction 2412345-100**

**Revision 1**

## ***GENIE Acquisition R4.0*** **Conformance Statement for DICOM v3.0**

**This document applies to the following systems:**

**Millennium MPR/MPS/MPT, MG and MC**

**MyoSIGHT**

**AC400**

**XC**

**XR**

**Copyright 2004 by General Electric Company**



---

**GE Medical Systems**

*GE Medical Systems: Telex 3797371  
P.O. Box 414, Milwaukee, Wisconsin, 53201 U.S.A.  
(Asia, Pacific, Latin America, North America)*

*GE Medical Systems -- Europe: Telex 698626  
283 rue de la Minière, B.P. 34, 78533, Buc Cedex, France*

## Revision History

Date	Name	Description Of Change	Revision
28 June 2004	Talia Cohen	Original	0.0
19 July 2003	Talia Cohen	Added Arnaud Gallois remarks	1.0

## TABLE OF CONTENTS

<b>1.</b>	<b>INTRODUCTION .....</b>	<b>1-1</b>
1.1	OVERVIEW .....	1-1
1.2	OVERALL DICOM CONFORMANCE STATEMENT DOCUMENT STRUCTURE.....	1-1
1.3	INTENDED AUDIENCE .....	1-3
1.4	SCOPE AND FIELD OF APPLICATION .....	1-3
1.5	IMPORTANT REMARKS .....	1-4
1.6	REFERENCES.....	1-4
1.7	DEFINITIONS.....	1-5
1.8	SYMBOLS AND ABBREVIATIONS .....	1-5
<b>2.</b>	<b>NETWORK CONFORMANCE STATEMENT .....</b>	<b>2-1</b>
2.1	INTRODUCTION.....	2-1
2.2	IMPLEMENTATION MODEL .....	2-2
2.3	AE SPECIFICATIONS .....	2-5
2.4	COMMUNICATION PROFILES.....	2-18
2.5	EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS .....	2-18
2.6	CONFIGURATION.....	2-19
2.7	SUPPORT OF EXTENDED CHARACTER SETS .....	2-20
<b>3.</b>	<b>NUCLEAR MEDICINE (NM) INFORMATION OBJECT IMPLEMENTATION .....</b>	<b>3-1</b>
3.1	introduction .....	3-1
3.2	NM IOD Implementation .....	3-1
3.3	NM Entity-Relationship Model.....	3-1
3.4	IOD MODULE TABLE.....	3-3
3.5	INFORMATION MODULE DEFINITIONS.....	3-4
3.6	PRIVate data dictionary .....	3-24
<b>4.</b>	<b>PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL DEFINITION .....</b>	<b>4-1</b>
4.1	introduction .....	4-1
4.2	Patient Root Information Model Description .....	4-1
4.3	Patient Root Information Model Entity-Relationship Model .....	4-1

4.4 INFORMATION Model Keys.....4-3

4.5 PRiVate data dictionary .....4-5

**5. STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL DEFINITION .....5-1**

5.1 introduction .....5-1

5.2 Study Root Information Model Description .....5-1

5.3 Study Root Information Model Entity-Relationship Model.....5-1

5.4 INFORMATION Model Keys.....5-3

5.5 PRiVate data dictionary .....5-5

**6. MODALITY WORKLIST INFORMATION MODEL DEFINITION..... 6-1**

6.1 INTRODUCTION.....6-1

6.2 MODALITY WORKLIST INFORMATION MODEL DESCRIPTION .....6-1

6.3 MODALITY WORKLIST INFORMATION MODEL ENTITY-RELATIONSHIP MODEL.....6-1

6.4 INFORMATION MODEL MODULE TABLE.....6-4

6.5 INFORMATION MODEL KEYS .....6-5

6.6 PRIVATE DATA DICTIONARY .....6-11

**7. XELERIS/ENTEGR A PROTOCOL DATA INFORMATION OBJECT DEFINITION ... 7-12**

7.1 INTRODUCTION.....7-12

7.2 Xeleris/eNTEGR A PROTOCOL DATA IOD IMPLEMENTATION.....7-12

7.3 IOD MODULE TABLE.....7-12

7.4 information module definitions.....7-13

7.5 PRiVate data dictionary .....7-17

**8. STORAGE COMMITMENT PUSH MODEL SOP CLASS DEFINITION ..... 8-18**

8.1 INTRODUCTION.....8-18

8.2 Storage Commitment PUSH Model SOP class definition.....8-18

8.2.1.1 STORAGE COMMITMENT MODULE .....8-18

**9. SECONDARY CAPTURE INFORMATION OBJECT IMPLEMENTATION ..... 9-22**

9.1 Secondary CAPTURE IOD MODULE TABLE.....9-22

9.2 INFORMATION MODULE DEFINITIONS.....9-22

9.3 Standard Extended and Private Data Attributes .....9-26

## LIST OF TABLES

TABLE 3.3-1 MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES .....	3-3
TABLE 3.4-1 NM IMAGE IOD MODULES .....	3-4
TABLE 3.5-1 PATIENT MODULE ATTRIBUTES .....	3-5
TABLE 3.5-2 GENIE ACQUISITION PATIENT MODULE ATTRIBUTES .....	3-5
TABLE 3.5-3 GENERAL STUDY MODULE ATTRIBUTES .....	3-6
TABLE 3.5-4 PATIENTS STUDY MODULE ATTRIBUTES .....	3-6
TABLE 3.5-5 GENIE ACQUISITION STUDY MODULE ATTRIBUTES.....	3-7
TABLE 3.5-6 GENERAL SERIES MODULE ATTRIBUTES.....	3-7
TABLE 3.5-7 GENIE ACQUISITION SERIES MODULE ATTRIBUTES .....	3-8
TABLE 3.5-8 FRAME OF REFERENCE MODULE ATTRIBUTES .....	3-9
TABLE 3.5-9 GENERAL EQUIPMENT MODULE ATTRIBUTES .....	3-10
TABLE 3.5-10 GENERAL IMAGE MODULE ATTRIBUTES .....	3-10
TABLE 3.5-11 GENIE ACQUISITION IMAGE MODULE ATTRIBUTES.....	3-11
TABLE 3.5-12 IMAGE PIXEL MODULE ATTRIBUTES .....	3-12
TABLE 3.5-13 GENIE ACQUISITION IMAGE PIXEL MODULE ATTRIBUTES.....	3-13
TABLE 3.5-14 MULTI-FRAME MODULE ATTRIBUTES.....	3-13
TABLE 3.5-15 SOP COMMON MODULE ATTRIBUTES.....	3-14
TABLE 3.5-16 NM/PET PATIENT ORIENTATION MODULE ATTRIBUTES .....	3-14
TABLE 3.5-17 NM IMAGE PIXEL MODULE ATTRIBUTES.....	3-15
TABLE 3.5-18 NM MULTI-FRAME MODULE ATTRIBUTES .....	3-15
TABLE 3.5-19 ENUMERATED VALUES FOR FRAME INCREMENT POINTER .....	3-16
TABLE 3.5-20 NM IMAGE MODULE ATTRIBUTES.....	3-16
TABLE 3.5-21 NM ISOTOPE MODULE ATTRIBUTES.....	3-18
TABLE 3.5-22 GENIE ACQUISITION ISOTOPE MODULE ATTRIBUTES.....	3-20
TABLE 3.5-23 NM DETECTOR MODULE ATTRIBUTES.....	3-20
TABLE 3.5-24 GENIE ACQUISITION DETECTOR MODULE ATTRIBUTES.....	3-21
TABLE 3.5-25 NM TOMO ACQUISITION MODULE ATTRIBUTES .....	3-21
TABLE 3.5-26 GENIE ACQUISITION TOMO ACQUISITION MODULE ATTRIBUTES .....	3-22
TABLE 3.5-27 NM MULTI-GATED ACQUISITION MODULE ATTRIBUTES .....	3-22
TABLE 3.5-28 GENIE ACQUISITION MULTI-GATED ACQUISITION MODULE ATTRIBUTES.....	3-23
TABLE 3.5-29 NM PHASE MODULE ATTRIBUTES .....	3-23
TABLE 3.6-1 PRIVATE CREATOR IDENTIFICATION (GEMS_GENIE_1) .....	3-24

DIR 2412345-100 REV 1

TABLE 4.3-1 MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES .....4-3

TABLE 4.4-1 PATIENT LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL .....4-4

TABLE 4.4-2 Q/R PATIENT LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES .....4-4

TABLE 4.4-3 STUDY LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL .....4-4

TABLE 4.4-4 Q/R STUDY LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES .....4-4

TABLE 4.4-5 SERIES LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL .....4-4

TABLE 4.4-6 Q/R SERIES LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES.....4-5

TABLE 4.4-7 IMAGE LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL.....4-5

TABLE 4.4-8 Q/R IMAGE LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES.....4-5

TABLE 5.3-1 MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES .....5-3

TABLE 5.4-1 STUDY LEVEL ATTRIBUTES FOR THE STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL.....5-3

TABLE 5.4-2 Q/R STUDY LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES .....5-4

TABLE 5.4-3 SERIES LEVEL ATTRIBUTES FOR THE STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL .....5-4

TABLE 5.4-4 Q/R SERIES LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES.....5-4

TABLE 5.4-5 IMAGE LEVEL ATTRIBUTES FOR THE STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL .....5-4

TABLE 5.4-6 Q/R IMAGE LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES.....5-4

TABLE 6.3-1 MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES .....6-4

TABLE 6.4-1 MODALITY WORKLIST INFORMATION MODEL MODULES .....6-4

TABLE 6.5-6.5-1 SOP COMMON MODULE ATTRIBUTES.....6-6

TABLE 6.5-6.5-2 SCHEDULED PROCEDURE STEP MODULE ATTRIBUTES.....6-6

TABLE 6.5-6.5-3 REQUESTED PROCEDURE MODULE ATTRIBUTES.....6-7

TABLE 6.5-6.5-4 IMAGING SERVICE REQUEST MODULE ATTRIBUTES .....6-8

TABLE 6.5-6.5-5 VISIT IDENTIFICATION MODULE ATTRIBUTES .....6-8

TABLE 6.5-6.5-6 VISIT STATUS MODULE ATTRIBUTES.....6-9

TABLE 6.5-6.5-7 VISIT RELATIONSHIP MODULE ATTRIBUTES .....6-9

TABLE 6.5-6.5-8 VISIT ADMISSION MODULE ATTRIBUTES .....6-9

TABLE 6.5-6.5-9 PATIENT RELATIONSHIP MODULE ATTRIBUTES .....6-9

TABLE 6.5-6.5-10 PATIENT IDENTIFICATION MODULE ATTRIBUTES .....6-10

TABLE 6.5-6.5-11 PATIENT DEMOGRAPHIC MODULE ATTRIBUTES .....6-10

TABLE 6.5-6.5-12 PATIENT MEDICAL MODULE ATTRIBUTES.....6-11

TABLE 7.3-1 XELERIS/ENTEGR A PROTOCOL DATA IOD MODULES.....7-13

TABLE 7.4-1 PATIENT MODULE ATTRIBUTES .....7-13

TABLE 7.4-1 GENIE ACQUISITION PATIENT MODULE ATTRIBUTES .....7-14

TABLE 7.4-1 GENERAL STUDY MODULE ATTRIBUTES .....7-14

TABLE 7.4-4 PATIENT STUDY MODULE ATTRIBUTES .....7-15

**GE MEDICAL SYSTEMS**

DIR 2412345-100 REV 1

**TABLE 7.4-4 GENIE ACQUISITION STUDY MODULE ATTRIBUTES.....7-15**

**TABLE 7.4-2 XELERIS/ENTEGR A PROTCOL DATA ATTRIBUTES .....7-16**

**TABLE 7.4-3 SOP COMMON MODULE ATTRIBUTES.....7-16**

**TABLE 7.5-1 PRIVATE CREATOR IDENTIFICATION (GEMS\_GENIE\_1) .....7-17**

**TABLE 9.1-1 SC IMAGE IOD MODULES .....9-22**

**TABLE 9.2-1 PATIENT IDENTIFICATION MODULE ATTRIBUES.....9-23**

**TABLE 9.2-2 GENERAL STUDY MODULE ATTRIBUTES.....9-23**

**TABLE 9-9.2-3 SC IMAGE EQUIPMENT MODULE ATTRIBUTES.....9-24**

**TABLE 9.2-4 IMAGE PIXEL MODULE ATTRIBUTES .....9-25**

**TABLE 9.2-5 SC IMAGE MODULE ATTRIBUTES .....9-26**

**TABLE 9.2-6 SOP COMMON MODULE ATTRIBUTES .....9-26**



# 1. INTRODUCTION

## 1.1 OVERVIEW

This DICOM Conformance Statement is divided into Sections as described below:

**Section 1 (Introduction)**, which describes the overall structure, intent, and references for this Conformance Statement

**Section 2 (Network Conformance Statement)**, which specifies the GEMS equipment compliance to the DICOM requirements for the implementation of Networking features.

**Section 3 (Nuclear Medicine Information Object Implementation)**, which specifies the GEMS equipment compliance to DICOM requirements for the implementation of a Nuclear Medicine Information Object.

**Section 4 (Patient Root Query/Retrieve Information Model Definition)**, which specifies the GEMS equipment compliance to DICOM requirements for the implementation of support for remote query/retrieve by patient of a Nuclear Medicine Information Object.

**Section 5 (Study Root Query/Retrieve Information Model Definition)**, which specifies the GEMS equipment compliance to DICOM requirements for the implementation of support for remote query/retrieve by study of a Nuclear Medicine Information Object.

**Section 6 (Modality Worklist Information Model Definition)**, which specifies the GEMS equipment compliance to DICOM requirements for the implementation of support for retrieving a worklist.

**Section 7. (Xeleris/eNTEGRA Protocol Data Information Object Implementation)** , which specifies the GEMS equipment compliance to DICOM requirements for the implementation of a private Xeleris/Entegra Protocol Data Information Object.


**Section 8. (Secondary Capture Information Object Implementation)**, which specifies the GEMS equipment compliance to DICOM requirements for the implementation of a Secondary Capture Information Object.

**Section 9. (Storage Commitment PUSH Model SOP Class definition)** which specifies the GEMS equipment compliance to DICOM requirements for the implementation of the Storage Commitment Push Model Service.

## 1.2 OVERALL DICOM CONFORMANCE STATEMENT DOCUMENT STRUCTURE


The Documentation Structure of the GEMS Conformance Statements and their relationship with the DICOM v3.0 Conformance Statements is shown in the Illustration below.

**ID/Net v3.0**




**APPLICATION ENTITY SPECIFICATION**  
 (SERVICE CLASSES, INFORMATION OBJECTS, MESSAGE EXCHANGES, ETC.)

**Product Implementation:**

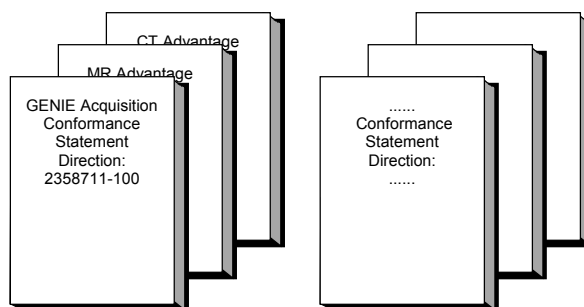

**DICOM STANDARD**

**Standard Specification:**

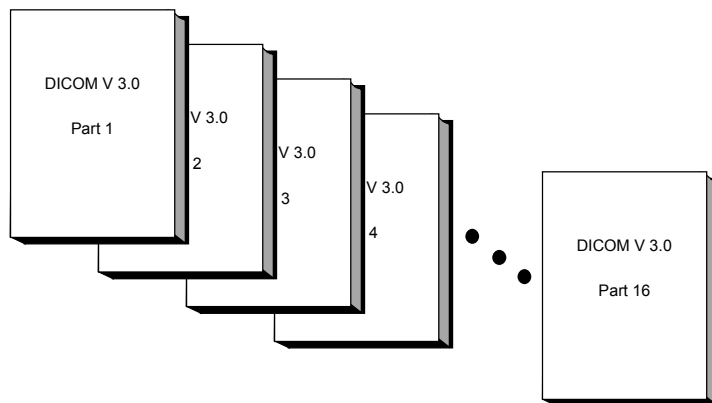

This document specifies the DICOM v3.0 implementation. It is entitled:

***GENIE Acquisition R4.0***  
*Conformance Statement for DICOM v3.0*  
*Direction 2358xxx-100*

This DICOM Conformance Statement documents the DICOM v3.0 Conformance Statement and Technical Specification required to interoperate with the GEMS network interface. Introductory information, which is applicable to all GEMS Conformance Statements, is described in the document:

*Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0)*  
*Conformance Statement*  
*Direction: 2118780.*

This Introduction familiarizes the reader with DICOM terminology and general concepts. It should be read prior to reading the individual products' GEMS Conformance Statements.

The GEMS Conformance Statement, contained in this document, also specifies the Lower Layer communications which it supports (e.g., TCP/IP). However, the Technical Specifications are defined in the DICOM v3.0 Part 8 standard.

For more information including Network Architecture and basic DICOM concepts, please refer to the Introduction.

For more information regarding DICOM, copies of the Standard may be obtained on the Internet at <http://medical.nema.org>. Comments on the standard may be addressed to: DICOM Secretariat

NEMA  
1300N. 17<sup>th</sup> Street, Suite 1847  
Rosslyn, VA 22209  
USA  
Phone: +1.703.841.3200

### 1.3 INTENDED AUDIENCE

The reader of this document is concerned with software design and/or system integration issues. It is assumed that the reader of this document is familiar with the DICOM v3.0 Standards and with the terminology and concepts which are used in those Standards.

If readers are unfamiliar with DICOM v3.0 terminology they should first refer to the document listed below, then read the DICOM v3.0 Standard itself, prior to reading this DICOM Conformance Statement document.

*Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0)*  
*Conformance Statement*  
*Direction: 2118780*

### 1.4 SCOPE AND FIELD OF APPLICATION

It is the intent of this document, in conjunction with the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*, to provide an unambiguous specification for GEMS implementations. This specification, called a Conformance Statement, includes a DICOM v3.0 Conformance Statement and is necessary to ensure proper processing and interpretation of GEMS medical data exchanged using DICOM v3.0. The GEMS Conformance Statements are available to the public.

The reader of this DICOM Conformance Statement should be aware that different GEMS devices are capable of using different Information Object Definitions. For example, a GEMS CT Scanner may send images using the CT Information Object, MR Information Object, Secondary Capture Object, etc.

Included in this DICOM Conformance Statement are the Module Definitions which define all data elements used by this GEMS implementation. If the user encounters unspecified private data elements while parsing a GEMS Data Set, the user is well

advised to ignore those data elements (per the DICOM v3.0 standard). Unspecified private data element information is subject to change without notice. If, however, the device is acting as a "full fidelity storage device", it should retain and re-transmit all of the private data elements which are sent by GEMS devices.

## 1.5 IMPORTANT REMARKS

The use of these DICOM Conformance Statements, in conjunction with the DICOM v3.0 Standards, is intended to facilitate communication with GE imaging equipment. However, **by itself, it is not sufficient to ensure that inter-operation will be successful.** The **user (or user's agent)** needs to proceed with caution and address at least four issues:

**Integration** - The integration of any device into an overall system of interconnected devices goes beyond the scope of standards (DICOM v3.0), and of this introduction and associated DICOM Conformance Statements when interoperability with non-GE equipment is desired. The responsibility to analyze the applications requirements and to design a solution that integrates GE imaging equipment with non-GE systems is the **user's** responsibility and should not be underestimated. The **user** is strongly advised to ensure that such an integration analysis is correctly performed.

**Validation** - Testing the complete range of possible interactions between any GE device and non-GE devices, before the connection is declared operational, should not be overlooked. Therefore, the **user** should ensure that any non-GE provider accepts full responsibility for all validation required for their connection with GE devices. This includes the accuracy of the image data once it has crossed the interface between the GE imaging equipment and the non-GE device and the stability of the image data for the intended applications.

Such a validation is required before any clinical use (diagnosis and/or treatment) is performed. It applies when images acquired on GE imaging equipment are processed/displayed on a non-GE device, as well as when images acquired on non-GE equipment is processed/displayed on a GE console or workstation.

**Future Evolution** - GE understands that the DICOM Standard will evolve to meet the user's growing requirements. GE is actively involved in the development of the DICOM v3.0 Standard. DICOM v3.0 will incorporate new features and technologies and GE may follow the evolution of the Standard. The GEMS protocol is based on DICOM v3.0 as specified in each ID/Net DICOM Conformance Statement. Evolution of the Standard may require changes to devices which have implemented DICOM v3.0. **In addition, GE reserves the right to discontinue or make changes to the support of communications features (on its products) reflected on by these ID/Net DICOM Conformance Statements.** The **user** should ensure that any non-GE provider, which connects with GE devices, also plans for the future evolution of the DICOM Standard. Failure to do so will likely result in the loss of function and/or connectivity as the DICOM Standard changes and GE Products are enhanced to support these changes.

**Interaction** - It is the sole responsibility of the **non-GE provider** to ensure that communication with the interfaced equipment does not cause degradation of GE imaging equipment performance and/or function.

## 1.6 REFERENCES

A list of references which is applicable to all GEMS Conformance Statements is included in the *Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780.*

The information object implementation refers to DICOM PS 3.3 (Information Object Definition).

## **1.7 DEFINITIONS**

A set of definitions which is applicable to all GEMS Conformance Statements is included in *the Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*.

## **1.8 SYMBOLS AND ABBREVIATIONS**

A list of symbols and abbreviations which is applicable to all GEMS Conformance Statements is included in *the Introduction to the Integrated DICOM/Network v3.0 (ID/Net v3.0) Conformance Statement, Direction: 2118780*.

**This Page Intentionally Left Blank**

## 2. NETWORK CONFORMANCE STATEMENT

### 2.1 INTRODUCTION

This section of the DICOM Conformance Statement specifies the compliance to DICOM conformance requirements for the relevant **Networking** features on this GEMS product. Note that the format of this section strictly follows the format defined in DICOM Standard PS 3.2 (Conformance). Please refer to that part of the standard while reading this section.

The GENIE Acquisition DICOM implementation allows the user to send Nuclear Medicine image data, acquired on GENIE Acquisition, to another DICOM station. For example, the user may wish to send data to a GENIE Processing and Review station in order to run the CEqual processing protocol. In this situation GENIE Acquisition is providing the DICOM C-STORE service as a service class user (SCU). GENIE Acquisition also allows query and retrieve of data stored in its local database from a remote station. In this situation GENIE Acquisition is providing the DICOM C-FIND and C-MOVE services as a service class provider (SCP).

The GENIE Acquisition DICOM implementation also provides a verification mechanism by which a remote application entity (AE) can verify application-level communication with the GENIE Acquisition DICOM Server. Also provided is a mechanism by which a GENIE Acquisition user can verify application-level communication with a remote DICOM AE. In these situations, GENIE Acquisition provides the DICOM C-ECHO service as both a SCP and SCU, respectively.

The GENIE Acquisition DICOM implementation can be configured to send Image data in a variety of formats. These formats allow the GENIE Acq to send data to an Xpert P&R, GENIE P&R, POWERstation as well as eNTEGRA and Xeleris. For example, the Xpert P&R expects multigated tomo data as an image per energy set per detector whereas the GENIE P&R expects an image per bin per energy set per detector. GENIE Acquisition can be configured to correct image data as part of the DICOM transfer.

GENIE Acquisition supports DICOM Modality Worklist as a service class user (SCU). The GENIE Acquisition worklist feature enables an operator to get their schedule of scans to perform directly from a Hospital/Radiology Information System (HIS/RIS). As well as providing a schedule of scans, the HIS/RIS also provides patient and study data. This reduces the operators' need for re-entering information already entered at the HIS/RIS.

GENIE Acquisition provides Ignite, a feature which allows a user to request a remote Xeleris station to process data. GENIE Acquisition implements this feature using a private Xeleris/eNTEGRA Protocol Data DICOM Information Object as a service class user (SCU). The GENIE Acquisition is configured with a list of processing protocols offered by one or more Xeleris stations. When defining an acquisition protocol or setting up a study, a user selects the processing protocols to be applied. After all the required data is acquired and transferred, a processing request is sent to the remote Xeleris station.

GENIE Acquisition supports DICOM Secondary Capture as a service class user (SCU). screen shots of part or all of the screen are captured and sent to remote station as DICOM secondary capture objects. A remote station can print and archive the secondary captures.

GENIE Acquisition supports DICOM Storage Commitment as a service class user (SCU). The Storage commitment feature enables a user to request a mass storage device or information system to take responsibility for acquisition data. A successful response will allow a user to delete the images knowing that they are still available on the network. The GENIE Acquisition operator can then safely delete the data knowing that it is still available elsewhere. Prior to this feature the operator was only told that data had been transferred off GENIE Acquisition.


## **2.2 IMPLEMENTATION MODEL**

All DICOM functionality on the GENIE Acquisition product is logically provided by the DICOM Server AE. The DICOM Server AE is commanded to perform DICOM services through the use of the GENIE Acquisition user interface. The DICOM Server AE also listens on a pre-defined port for incoming connections from remote DICOM AEs.

### **2.2.1 Application Data Flow Diagram**

The Basic and Specific Application models for this device are shown in the following illustration :



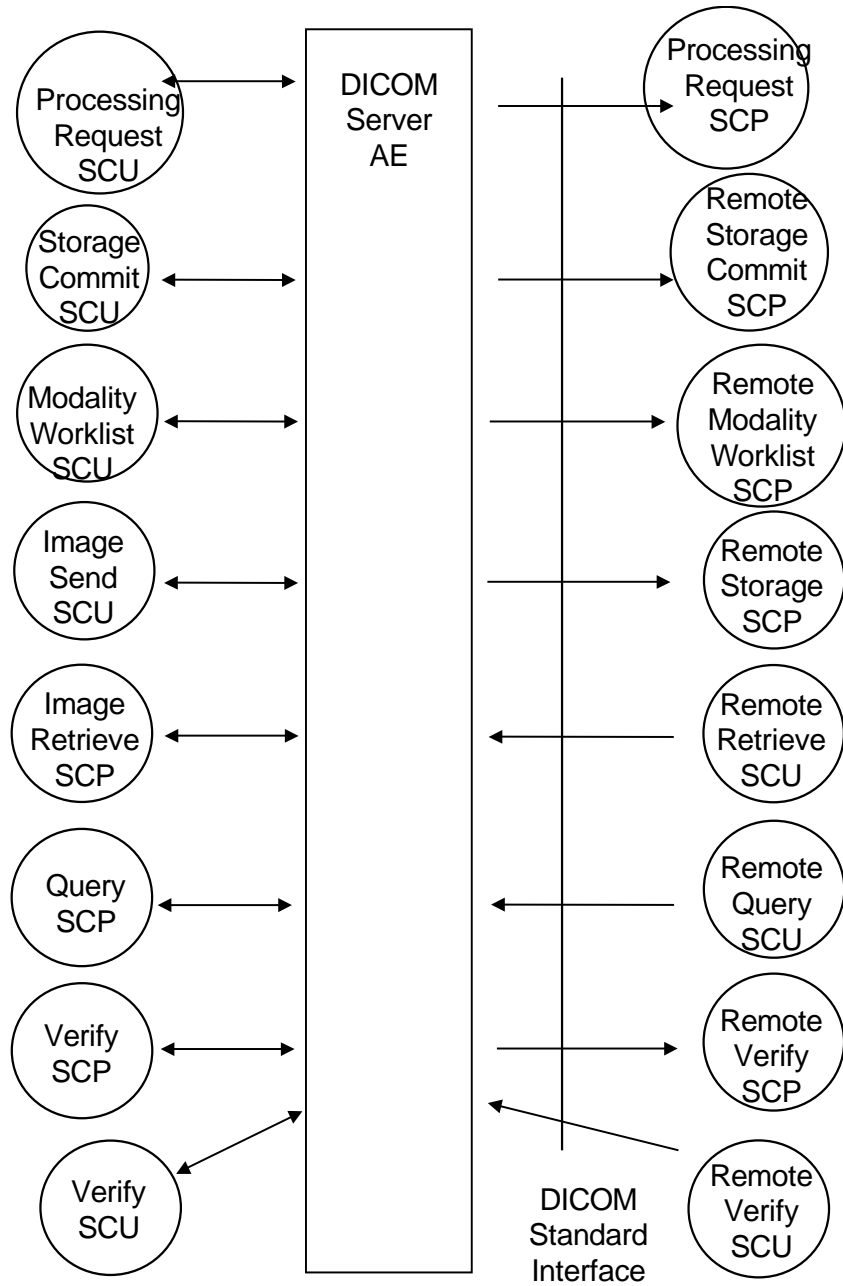

## 2.2.2 Functional Definition of AE's

The GENIE Acquisition DICOM Server AE initiates the following functions:

*Worklist:* Initiates a DICOM association in order to retrieve a list of scans to perform from the remote AE. Issues a C-FIND-RQ for DICOM Scheduled Procedure Steps and waits for C-FIND-RSP messages. The first C-FIND-RSP contains a match and a status of "pending". All other matches are also returned in C-FIND-RSP messages with status "pending" until the last message which is returned with a final status of "success", "warning" or "failure".

*Store:* Initiates a DICOM association in order to send acquired or screen capture images to a remote AE. If the remote AE accepts a presentation context applicable to the image(s) being sent, the DICOM Server will send the images via the C-STORE service.

*Verify:* Initiates a DICOM association in order to send a verification message to a remote AE via a C-ECHO-RQ message.

*Commitment:* Initiates a DICOM Storage Commitment request once a Store request has completed successfully. An N-ACTION request specifying all the successfully transferred images will be issued to the remote AE. The remote AE will reply accepting or refusing the request. If accepted the remote AE will issue an N-EVENT response specifying which images have been committed and which, if any, have not.

*Protocol Data:* Initiates a DICOM association in order to request processing on a remote AE. If the remote AE accepts a presentation context for the private Xeleris/eNTEGRA protocol data, the DICOM Server will send the processing request via the C-STORE service. No confirmation of actual processing is received.

The GENIE Acquisition DICOM Server AE responds to the following functions:

*Query:* Accepts a DICOM association initiated remotely in order to receive a C-FIND-RQ. Responds to incoming C-FIND-RQ messages by searching its local database for the requested attributes and returning a C-FIND-RSP message containing a match and a status of "pending." All other matches are also returned in C-FIND-RSP messages with status of "pending" until the last message which is returned with a final status of "success", "warning" or "failure". The remote AE can terminate the query by sending a C-CANCEL-FIND-RQ message.

*Retrieve:* Accepts a DICOM association initiated remotely in order to receive a C-MOVE-RQ. Responds to incoming C-MOVE-RQ messages by searching its local database for the requested image(s) and returning each via a C-STORE-RQ message. The DICOM Server will return a C-FIND-RSP message after each image is sent. The status returned is "pending" until the last image is sent, in which case the appropriate status is returned. The remote AE can terminate the retrieve by sending a C-CANCEL-MOVE-RQ message.

*Verify:* Accepts a DICOM association initiated remotely in order to receive a C-ECHO-RQ. Responds to incoming C-ECHO-RQ messages by returning a C-ECHO-RSP message with a status of "success."

## 2.2.3 Sequencing of Real-World Activities

Non Applicable.

**2.3.1 DICOM Server AE Specification**

This Application Entity provides Standard Conformance to the following DICOM v3.0 SOP Classes as an **SCU**:

SOP Class Name	SOP Class UID
Modality Worklist Information Model – FIND	1.2.840.10008.5.1.4.31
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Verification	1.2.840.10008.1.1
Storage Commitment Push Model	1.2.840.10008.1.20.1
Xeleris/eNTEGRA Protocol Data	1.2.840.113619.4.27

This Application Entity provides Standard Conformance to the following DICOM v3.0 SOP Classes as an **SCP**:

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2
Verification	1.2.840.10008.1.1

**2.3.1.1 Association Establishment Policies**

**2.3.1.1.1 General**

The DICOM Application Context Name (ACN), which is always proposed, is:

<b>Application Context Name</b>	<b>1.2.840.10008.3.1.1.1</b>
---------------------------------	------------------------------

The Maximum Length PDU negotiation is included in all association establishment requests. The maximum length PDU for an association initiated by the DICOM Server is:

<b>Maximum Length PDU</b>	<b>10038 bytes</b>
---------------------------	--------------------

The SOP Class Extended Negotiation is not supported.

The maximum number of Presentation Context Items that will be proposed is 8. Note that the same Abstract Syntax may be offered multiple times with different Transfer Syntaxes.

The user information Items sent by this product are:

- Maximum PDU Length
- Implementation UID

**2.3.1.1.2 Number of Associations**

The DICOM Server AE (SCU) will initiate only one DICOM association at a time to a single remote AE. A configurable number (default 2) of simultaneous DICOM associations can be open to different remote AEs. An individual association may be used either for querying worklists or for storing images.

The DICOM Server AE (SCP) can have a configured number (default 4) of DICOM associations open to service queries, retrieves or verifications.

**2.3.1.1.3 Asynchronous Nature**

Asynchronous mode is not supported. All operations are performed synchronously.

**2.3.1.1.4 Implementation Identifying Information**

The Implementation UID for this DICOM v3.0 Implementation is:

<b>GENIE Acquisition Implementation UID</b>	<b>1.2.840.113619.6.175</b>
---	-----------------------------

**2.3.1.2 Association Initiation Policy**

The DICOM Server AE initiates a new association due to an acquired or screen capture image send, worklist query, processing request or storage commitment operation being initiated from the GENIE Acquisition user interface or due to image data being retrieved by a remote AE. The DICOM Server AE also initiates a new association when the operator initiates a verification operation via the utility “DICOMping.”

### **2.3.1.2.1 Real-World Activity: Modality Worklist Query SCU**

#### **2.3.1.2.1.1 Associated Real-World Activity**

The operator must specify the query by which a remote MWL (SCP) performs matching.

The operator can specify matching by:

Scheduled Station AE title

Scheduled Station Name

Scheduled Procedure Step Start Date

Modality

In addition, the operator can further qualify a query by one of:

Scheduled Procedure Step ID

Requested Procedure ID

Accession Number

Patient Name and/or Patient ID

The application will complete a query containing a Date by specifying a Scheduled Procedure Step Start Time range of daybreak to midnight.

Once the query has been specified, the operator pushes the “Query” button to initiate the MWL query operation. The DICOM Server will then initiate an association with the remote AE in order to send the query and receive the matching worklist entries.

Each Worklist response can be browsed to review most of their attributes. Some attributes do not have an operator meaning and cannot be reviewed, e.g Study DICOM UID.

A Worklist response that is to be scanned, can be selected and added to the “ToDo” list. The application now proceeds in the same way as for non-worklist created “ToDo” entries.

A single association is used to send the query and receive all the matches.

**2.3.1.2.1.2 Proposed Presentation Context Table**

The following table shows the proposed presentation contexts for the DICOM Server AE after real-world activity “Modality Worklist” has been initiated:

Presentation Context Table – Proposed					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Modality Worklist Information Model – FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

**2.3.1.2.1.2.1 SOP Specific DICOM Conformance Statement for the Modality Worklist SOP Classes**

Upon receiving a C-FIND confirmation containing a Refused status, this implementation will terminate the association.

A C-FIND request can result in multiple C-FIND responses over a single association.

Following are the status codes that are more specifically processed when receiving messages from **Modality Worklist** SCP equipment:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Refused	A700	Out of resources	Error logged and dialog displayed to user.
Failed	Cxxx	Unable to process	Error logged and dialog displayed to user.
Cancel	FE00	Matching terminated due to cancel	A user request to cancel the query has been actioned and is acknowledged. Cancel logged.
Success	0000	Matching is complete - No final identifier is supplied	
Pending	FF00	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys.	Continue receiving matches and displaying them in the Scheduled Procedure Step browser.
	FF01	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this Identifier	Continue receiving matches and displaying them in the Scheduled Procedure Step browser.

**2.3.1.2.2 Real-World Activity: Image Send SCU**

**2.3.1.2.2.1 Associated Real-World Activity**

To transfer acquired images the operator must both select image(s) from the Patient Selector and a destination from the Network Card. Once these selections have been made, the operator pushes the “Send” button to initiate an acquired image send operation. The DICOM Server will then initiate an association with the remote AE in order to send the selected acquired image(s). A single association is used to send all data for a single destination.

Image Send activity is also initiated by Image Retrieve activity.

Secondary capture image printing results in image send. The operator can capture areas of the screen through the user interface. These screen captures are automatically sent to the configured print device which can be a remote DICOM station. The DICOM Server will initiate an association with the remote AE in order to send the screen captures.

**2.3.1.2.2.2 Proposed Presentation Context Table**

The following table shows the proposed presentation contexts for the DICOM Server AE after real-world activity “Image Send” has been initiated:

<b>Presentation Context Table – Proposed</b>					
<b>Abstract Syntax</b>		<b>Transfer Syntax</b>		<b>Role</b>	<b>Extended Negotiation</b>
<b>Name</b>	<b>UID</b>	<b>Name List</b>	<b>UID List</b>		
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

**2.3.1.2.2.2.1 SOP Specific DICOM Conformance Statement for all Storage SOP Classes**

This implementation can perform multiple C-STORE operations over a single association.

Upon receiving a C-STORE confirmation containing a Successful status, this implementation will perform the next C-STORE operation. The association will be maintained if possible.

Upon receiving a C-STORE confirmation containing a Refused status, this implementation will terminate the association.

Upon receiving a C-STORE confirmation containing a status other than Successful or Refused, this implementation will consider the current request to be a failure but will continue to attempt to send any remaining images in the request using the same association.

If any timers expire, the association is closed and the operation in progress is considered to be failed.

Following are the status codes that are more specifically processed when receiving messages from **Storage SCP** equipment:

<b>Service Status</b>	<b>Status Codes</b>	<b>Further Meaning</b>	<b>Application Behavior When receiving Status Codes</b>
Refused	A7xx	Out of resources	The message "Sent I of J : K Failed" is posted to the Log card. I and K are incremented such that I equal J and K are incremented by the same amount.
	0122	SOP Class not Supported	The message "Sent I of J : K Failed" is posted to the Log card. I and K are incremented such that I equal J and K are incremented by the same amount.
Error	Cxxx	Cannot Understand	The message "Sent I of J : K Failed" is posted to the Log card. I and K are incremented by one
	A9xx	Data Set does not match SOP Class	The message "Sent I of J : K Failed" is posted to the Log card. I and K are incremented by one.
Warning	B000	Coercion of Data Elements	The message "Sent I of J : K Failed" is posted to the Log card. I and K are incremented by one
	B007	Data Set does not match SOP Class	The message "Sent I of J : K Failed" is posted to the Log card. I and K are incremented by one
	B006	Elements Discarded	The message "Sent I of J : K Failed" is posted to the Log card. I and K are incremented by one
Success	0000		The message "Sent I of J : K Failed" is posted to the Log card. I is incremented by one



**2.3.1.2.3 Real-World Activity: Verify SCU**

**2.3.1.2.3.1 Associated Real-World Activity**

Service personnel invoke the utility “DICOMping” from the UNIX command line. The AE Title of the remote is supplied on the command line. The DICOM server will initiate an association with the remote DICOM AE in order to verify communication at the application level. The success or failure of the verification process is displayed to the user.

The IP and port number for the echo SCP is retrieved from a configuration file.

**2.3.1.2.3.2 Proposed Presentation Context Table**

Presentation Context Table - Proposed					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification SOP Class	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

**2.3.1.2.3.2.1 SOP Specific DICOM Conformance Statement for Verification SOP Class**

The DICOM Server AE provides standard conformance to the DICOM Verification Service Class.

**2.3.1.2.4 Real-World Activity: Storage Commitment SCU**

**2.3.1.2.4.1 Associated Real-World Activity**

The operator must both select image(s) to be transferred from the Patient Selector and select a destination from the Network Card that provides Storage Commitment. Once these selections have been made, the operator pushes the “Send” button to initiate an image send operation. The DICOM Server will then initiate an association with the remote AE in order to send the selected image(s). A single association is used to send all data for a single destination.

If one or more images are successfully transferred the DICOM server will initiate a new association and issue a storage commitment request for the successfully transferred images. The new association can be to a different remote AE as the one sent the images. The original association will be closed. The status of the images will be updated to show that a storage commitment request has been made.

Some time later the remote Storage Commitment server will initiate an association to the DICOM server and issue a storage commitment result. The DICOM server will receive the result and update the status of the images for which the result relates.

**2.3.1.2.4.2 Proposed Presentation Context Table**

The following table shows the proposed presentation contexts for the DICOM Server AE after real-world activity “Storage Commit” has been initiated.

Presentation Context Table – Proposed					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

**2.3.1.2.4.3 SOP Specific Conformance Statement for the Storage Commitment Push Model SOP Class**

This implementation issues one N-ACTION request for storage commitment per set of C-STORE requests performed across a single association. Only C-STORE requests that result in a C-STORE response of success and performed to a specific storage commitment SCP will be considered for storage commitment. The attributes of the request will identify the NM image objects for which commitment is being requested. The referenced Study Component Sequence and Storage Media File-Set ID and UID attributes are not supported.

Upon receiving an N-ACTION response this implementation will close the association. This implementation will then wait for an N-EVENT-REPORT response from the SCP. If further storage commitment requests are made on all of the referenced SOP instances then this implementation will no longer wait for the N-EVENT-REPORT response.

No service class specific status values are defined for the N-ACTION Service. See PS 3.7 for general response status codes.

When the Storage Commitment SCP is ready it will open an association to this implementation and send an N-EVENT-REPORT request. The attributes of the request will identify the NM image objects for which commitment has succeeded and those for which it has failed. No further DICOM actions will be taken.

No service class specific status values are defined for the N-EVENT report service. See PS 3.7 for general response status codes.

**2.3.1.2.5 Real-World Activity: Xeleris/eNTEGRA Protocol Data**

**2.3.1.2.5.1 Associated Real-World Activity**

When defining an acquisition protocol or setting up a study, the GENIE Acq user selects the processing protocols to be applied. After all the required data is acquired and transferred to a remote station, GENIE Acquisition sends a processing request to remote AE using C-STORE command.

**2.3.1.2.5.2 Proposed Presentation Context Table**

The following table shows the proposed presentation contexts for the DICOM Server AE after real-world activity “Xeleris/eNTEGRA Protocol Data” has been initiated.

Name	UID	Name List	UID List	Role	Extended Negotiation
Xeleris/eNTEGRA Protocol Data	1.2.840.113619.4.27	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

**2.3.1.2.5.3 SOP Specific Conformance statement for the Xeleris/eNTEGRA Protocol Data SOP Class**

The DICOM Server AE conforms to the DICOM Storage Service Class for sending GEMS Private Xeleris/eNTEGRA Protocol Data Information Objects.

The implementation is equivalent to that for sending images (See 2.3.1.2.2.1 SOP Specific DICOM Conformance Statement for all Storage SOP Classes)

**2.3.1.2.6 Real-World Activity: Query SCP**

**2.3.1.2.6.1 Associated Real-World Activity**

The DICOM Server AE is always listening for associations. No operator action is required to respond to Query request.

The real-world activity associated with the Query request is to search the local database for all entries that match the request and send a C-FIND-RSP message with the status of “pending” for each matching entry. The exception to this is the last message which is sent with a status of “success”, “failure” or “refused”.

2.3.1.2.6.2 Accepted Presentation Context Table

Presentation Context Table – Accepted					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Note that this implementation does not support extended negotiation for the C-FIND Service, including that for relational-queries.

2.3.1.2.6.2.1 SOP Specific DICOM Conformance Statement for the Patient Root Query/Retrieve Information Model - FIND and Study Root Query/Retrieve Information Model - FIND SOP Classes

Following are the status codes the Application may send back to the SCU Equipment after performing the requested Query :

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Refused	A700	Out of resources	
Failed	C000	Unable to process	Returned by the DICOM Server if for any other reason, not specified elsewhere in this table, the Find operation failed; error logged.
Cancel	FE00	Matching terminated due to cancel	Returned if the DICOM Server receives a C-CANCEL-FIND-RQ message; cancel logged.
Success	0000	Matching is complete - No final identifier is supplied	Returned when the DICOM Server completes the find operation.
Pending	FF00	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys.	
	FF01	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this Identifier	

2.3.1.2.6.3 Presentation Context Acceptance Criterion

The Presentation Contexts that will be accepted by the DICOM Server will be the ones which the remote SCU has requested and that are supported by the GENIE Acquisition.

2.3.1.2.6.4 Transfer Syntax Selection Policies

In the case that multiple transfer syntaxes are requested for a single Presentation Context then GENIE Acquisition selects the one which is listed first in the accepted presentation context table specified above.

**2.3.1.2.7 Real-World Activity: Image Retrieve SCP**

**2.3.1.2.7.1 Associated Real-World Activity**

The DICOM Server AE is always listening for associations. No operator action is required to respond to an Image Retrieve request.

The real-world activity associated with the Image Retrieve request is to send all images corresponding to the C-MOVE request to the specified destination AE through a separate association.

**2.3.1.2.7.2 Accepted Presentation Context Table**

Presentation Context Table – Accepted					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Note that this implementation does not support extended negotiation for the C-MOVE Service, including that for relational-retrieve.

**2.3.1.2.7.2.1 SOP Specific DICOM Conformance Statement for the Patient Root Query/Retrieve Information Model - MOVE and Study Root Query/Retrieve Information Model - MOVE SOP Classes**

Following are the status codes the Application may send back to the SCU Equipment after performing the requested **Retrieve** :

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Refused	A701	Out of resources - Unable to calculate number of matches	
	A702	Out of resources - Unable to perform sub-operations	
	A801	Move Destination Unknown	Returned if the DICOM Server has no information on destination AE; error logged.
Failed	A900	Identifier does not match SOP Class	
	C000	Unable to process	Returned by the DICOM Server if for any other reason, not specified elsewhere in this table, the Find operation failed; error logged.
Cancel	FE00	Sub-operations terminated due to a Cancel indication	Returned if the DICOM Server receives a C-CANCEL-MOVE-RQ message.
Warning	B000	Sub-operations Complete - One or more Failures.	Returned upon completion if one or more of the specified images failed to transfer to the destination AE.
Success	0000	Sub-operations Complete - No Failure	Returned after the transfer of the last image.
Pending	FF00	Sub-operations are continuing	Returned after the transfer of each image except for the last.

#### **2.3.1.2.7.3 Presentation Context Acceptance Criterion**

The Presentation Contexts that will be accepted by the DICOM Server will be the ones which the remote SCU has requested and that are supported by the GENIE Acquisition.

#### **2.3.1.2.7.4 Transfer Syntax Selection Policies**

In the case that multiple transfer syntaxes are requested for a single Presentation Context then GENIE Acquisition selects the one which is listed first in the accepted presentation context table specified above.

**2.3.1.2.8 Real-World Activity: Verify SCP**

**2.3.1.2.8.1 Associated Real-World Activity**

The DICOM Server AE is always listening for associations. No operator action is required to respond to a Verification request.

The real-world activity associated with the Verification request is to send a C-ECHO-RSP message with a status of “success” to the requesting AE.

**2.3.1.2.8.2 Accepted Presentation Context Table**

<b>Presentation Context Table - Accepted</b>					
<b>Abstract Syntax</b>		<b>Transfer Syntax</b>		<b>Role</b>	<b>Extended Negotiation</b>
<b>Name</b>	<b>UID</b>	<b>Name List</b>	<b>UID List</b>		
Verification SOP Class	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

**2.3.1.2.8.2.1 SOP Specific DICOM Conformance Statement for Verification SOP Class**

The DICOM Server AE provides standard conformance to the DICOM verification service class.

**2.3.1.2.8.3 Presentation Context Acceptance Criterion**

The Presentation Contexts that will be accepted by the DICOM Server will be the ones which the remote SCU has requested and that are supported by the GENIE Acquisition.

**2.3.1.2.8.4 Transfer Syntax Selection Policies**

In the case that multiple transfer syntaxes are requested for a single Presentation Context then GENIE Acquisition selects the one which is listed first in the accepted presentation context table specified above.

## **2.4 COMMUNICATION PROFILES**

### **2.4.1 Supported Communication Stacks (PS 3.8, PS 3.9)**

DICOM Upper Layer (PS 3.8) is supported using TCP/IP.

### **2.4.2 OSI Stack**

The OSI Communication Stack is not supported by this implementation.

### **2.4.3 TCP/IP Stack**

The TCP/IP Communication Stack is inherited from the LynxOS real-time unix operating system.

#### **2.4.3.1 API**

Not applicable to this product.

#### **2.4.3.2 Physical Media Support**

DICOM is indifferent to the Physical medium over which TCP/IP executes (e.g. Ethernet V2.0, IEEE 802.3, ATM, FDDI)

Note: For more information about the Physical Media available on GENIE Acquisition, please refer to the Product Data Sheet.

### **2.4.4 Point-to-Point Stack**

The Point-to-Point Communication Stack is not supported by this implementation.

## **2.5 EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS**

### **2.5.1 Standard Extended /Specialized/Private SOPs**

GENIE Acquisition implements the extended SOP class object NM IOD (see section 3) and the GEMS Private SOP class object Xeleris/eNTEGRA Protocol Data IOD (see section 7)

### **2.5.2 Private Transfer Syntaxes**

GENIE Acquisition does not implement any private transfer syntaxes.



The GENIE Acquisition system is configured by GEMS Field Service Engineers. The DICOM configuration items below are configurable or re-configurable by a Field Service Engineer but are not accessible through the GENIE Acquisition user interface.

**2.6.1 AE Title/Presentation Address Mapping**

GENIE Acquisition allows for the configuration of the mapping of remote AE titles to IP addresses and ports. This configuration is performed by GEMS Field Service Engineers.

**2.6.2 Configurable Parameters**

The following parameters are configurable for the DICOM Server AE:

- Local AE Title (set to hostname of GENIE Acquisition computer)
- Local IP address
- Local IP netmask
- Local IP gateway

Note that the port on which GENIE Acquisition receives DICOM incoming TCP/IP connections is **2030**.

The following fields are configurable for every remote DICOM AE:

- Remote AE Title
- Remote IP Address
- Listening TCP/IP Port Number

A default router can be defined to reach remote stations.

The following fields are configurable:

- Association Establishment Timer
- Store, Find, Move, Timers
- Inactivity Timers
- Maximum Length PDU
- Number of simultaneous associations

Note: All configurations must be performed by a GE Field Engineer.

**2.6.2.1 Inactivity Timers**

The table below specifies all of the timeouts that can be configured by a GE Field Service Engineer:

<b>Timeout</b>	<b>Default (Seconds)</b>	<b>Note</b>
Session	7200	This timer starts when an connection request is sent or received. The timer end either through timeout or when the connection is closed.
Association	60	Association inactivity timeout. Used when no operation is in progress.
Abort	60	Physical connection close timeout under abnormal conditions.
C-ECHO	20	Operation inactivity timeout
C-STORE	3600	Operation inactivity timeout
C-FIND	3600	Operation inactivity timeout
C-MOVE	3600	Operation inactivity timeout
N-CREATE	3600	Operation inactivity timeout
N-DELETE	3600	Operation inactivity timeout
N-SET	3600	Operation inactivity timeout
N-GET	3600	Operation inactivity timeout
N-ACTION	3600	Operation inactivity timeout
N-EVENT	3600	Operation inactivity timeout

**2.7 SUPPORT OF EXTENDED CHARACTER SETS**

GENIE Acquisition will support only the ISO\_IR 100 (ISO 8859-1:1987 Latin alphabet N 1. supplementary set) as extended character sets.

**This Page Intentionally Left Blank**

### **3. NUCLEAR MEDICINE (NM) INFORMATION OBJECT IMPLEMENTATION**

#### **3.1 INTRODUCTION**

This section specifies the use of the DICOM NM Image IOD to represent the information included in NM images produced by this implementation. Corresponding attributes are conveyed using the module construct. The contents of this section are:

- 3.2 - IOD Description
- 3.3 - IOD Entity-Relationship Model
- 3.4 - IOD Module Table
- 3.5 - IOD Module Definition

#### **3.2 NM IOD IMPLEMENTATION**

The GENIE Acquisition implementation of DICOM uses the Nuclear Medicine multi-frame image format when creating image objects. In order to preserve full fidelity when transferring data to a GENIE Processing and Review station, some specialized database information is encoded as private DICOM attributes. The private data dictionary is included in section 3.6.

Note that the GENIE Acquisition DICOM implementation creates separate NM images (SOP instances) for each energy window (energy set) in the acquisition. It may also create separate images (SOP instances) for each detector in the acquisition.

#### **3.3 NM ENTITY-RELATIONSHIP MODEL**

The Entity-Relationship diagram for the NM Image interoperability schema is shown in Figure 3-1. In this figure, the following diagrammatic convention is established to represent the information organization :


- each entity is represented by a rectangular box.
- each relationship is represented by a diamond shaped box.
- the fact that a relationship exists between two entities is depicted by lines connecting the corresponding entity boxes to the relationship boxes.

The relationships are fully defined with the maximum number of possible entities in the relationship shown. In other words, the relationship between Series and Image can have up to n Images per Series, but the Patient to Study relationship has 1 Study for each Patient (a Patient can have more than one Study on the system, however, each Study will contain information pertaining to that one Patient).

DIR 2412345-100 REV 1

FIGURE 3-1

NM IMAGE ENTITY RELATIONSHIP DIAGRAM

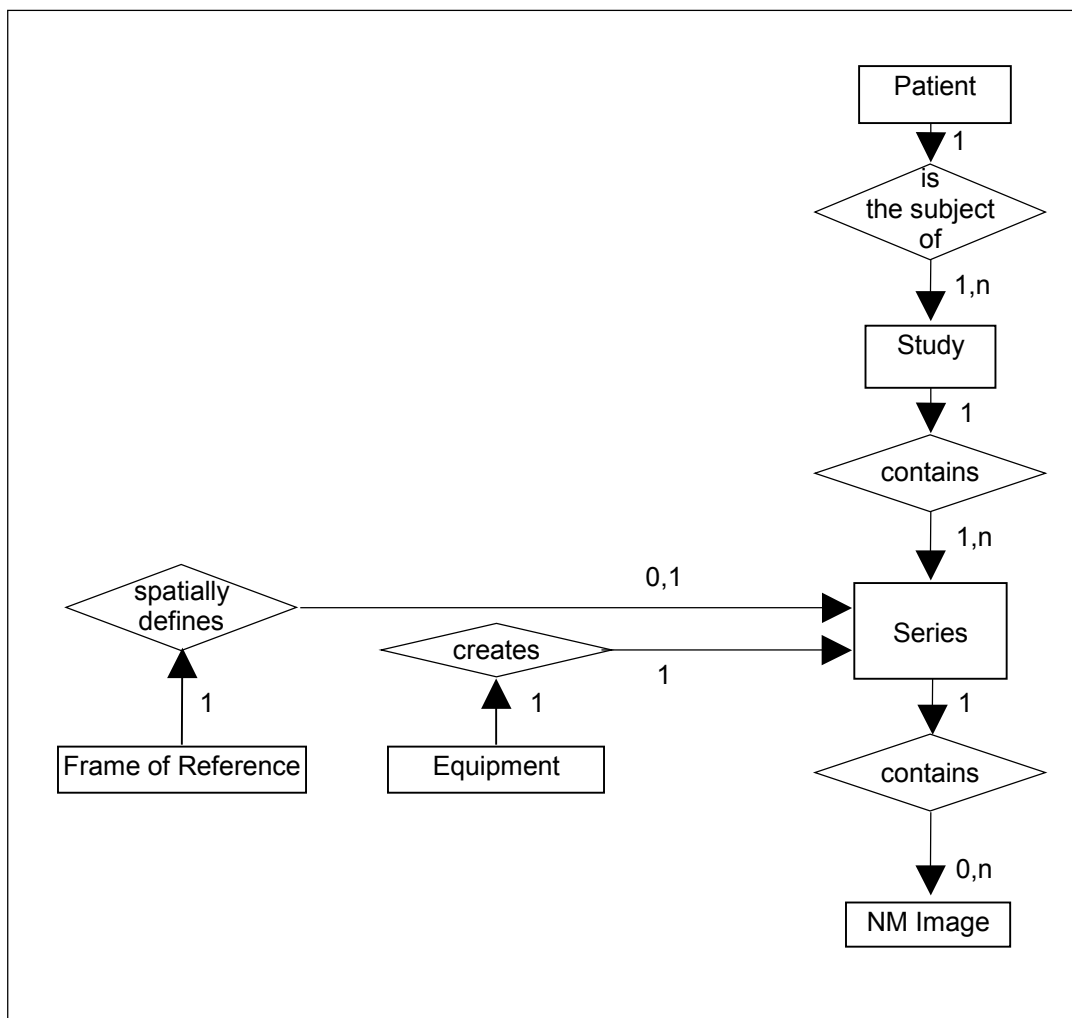

**3.3.1 ENTITY DESCRIPTIONS**

Please refer to DICOM Standard Part 3 (Information Object Definitions) for a description of each of the entities contained within the NM Information Object.

**3.3.1.1 Patient Entity Description**

The Patient Entity defines the characteristics of a patient who is the subject of one or more medical studies which produce medical images.

**3.3.1.2 Study Entity Description**

The Study Entity defines the characteristics of a medical study performed on a patient. A study is a collection of one or more series of medical images which are logically related for the purpose of diagnosing a patient. Each study is associated with exactly one patient.

**3.3.1.3 Series Entity Description**

The Series Entity defines the attributes which are used to group images into distinct logical sets. Each series is associated with exactly one study.

**3.3.1.4 Equipment Entity Description**

The Equipment Entity describes the particular imaging device which produced the series of images. An imaging device may produce one or more series within a study. The Equipment Entity does not describe the data acquisition or image creation Attributes used to generate images within a series.

**3.3.1.5 Frame of Reference Entity Description**

The Frame of Reference Entity identifies the coordinate system which conveys spatial and/or temporal information of images in a series.

**3.3.1.6 NM Image Entity Description**

The NM Image Entity defines the attributes which describe the pixel data of a NM image. The pixel data is generated on GENIE Acquisition as a direct result of patient scanning (an Original image). An image is defined by its image plane, pixel data characteristics, gray scale and/or color mapping characteristics and modality specific characteristics (acquisition parameters and image creation information).

**3.3.2 GENIE Acquisition Mapping of DICOM entities**

**TABLE 3.3-1  
MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES**

DICOM	GENIE Acquisition Entity
Patient	Patient
Study	Study
Series	Series
Image	Imageset
Frame	Not Applicable

**3.4 IOD MODULE TABLE**

Within an entity of the DICOM v3.0 NM IOD, attributes are grouped into related sets of attributes. A set of related attributes is termed a module. A module facilitates the understanding of the semantics concerning the attributes and how the attributes are related to each other. A module grouping does not infer any encoding of information into datasets.

Table 3.4-1 identifies the defined modules within the entities which comprise the DICOM v3.0 NM IOD. Modules are identified by Module Name.

Please refer to the DICOM v3.0 Standard Part 3 for a complete definition of the entities, modules, and attributes.

Entity Name	Module Name	Reference
Patient	Patient	3.5.1.1
	GENIE Acquisition Patient	3.5.1.2
Study	General Study	3.5.2.1
	Patient Study	3.5.2.2
	GENIE Acquisition Study	3.5.2.3
Series	General Series	3.5.3.1
	GENIE Acquisition Series	3.5.3.2
	NM/PET Patient Orientation	3.5.8.1
Frame of Reference	Frame of Reference	3.5.4.1
Equipment	General Equipment	3.5.5.1
Image	General Image	3.5.6.1
	GENIE Acquisition Image	3.5.6.2
	Image Pixel	3.5.6.3
	NM Image Pixel	3.5.8.2
	GENIE Acquisition Image Pixel	3.5.6.4
	Multi-frame	3.5.6.5
	NM Multi-frame	3.5.8.3
	NM Image	3.5.8.4
	NM Isotope	3.5.8.5
	GENIE Acquisition Isotope	3.5.8.5.1
	NM Detector	3.5.8.7
	GENIE Acquisition Detector	3.5.8.8
	NM TOMO Acquisition	3.5.8.9
	GENIE Acquisition TOMO Acquisition	3.5.8.10
	NM Multi-gated Acquisition	3.5.8.11
	GENIE Acquisition Multi-gated Acquisition	3.5.8.12
	NM Phase	3.5.8.13
	NM Reconstruction	Not used.
	Overlay Plane	Not used.
	Multi-frame overlay	Not used.
Curve	Not used.	
VOI LUT	Not used.	
SOP Common	3.5.7.1	

**3.5 INFORMATION MODULE DEFINITIONS**

Please refer to the DICOM v3.0 Standard Part 3 (Information Object Definitions) for a description of each of the entities and modules contained within the NM Information Object.

The following modules are included to convey Enumerated Values, Defined Terms, and Optional Attributes supported. Type 1 & Type 2 Attributes are also included for completeness and to define what values they may take and where these values are obtained from. It should be noted that they are the same as those defined in the DICOM v3.0 Standard Part 3 (Information Object Definitions).

3.5.1 Common Patient Entity Modules

3.5.1.1 Patient Module

This section specifies the Attributes of the patient that describe and identify the patient who is the subject of a diagnostic Study. This Module contains Attributes of the patient that are needed for diagnostic interpretation of the Image and are common for all studies performed on the patient.

TABLE 3.5-1  
PATIENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Patient's Name	(0010,0010)	2	Entered on To Do card, Patient Name field, or filled-in from worklist. Name is sent with PN VR individual component values if entered that way.
Patient ID	(0010,0020)	2	Entered on To Do card, Patient ID field, or filled-in from worklist.
Patient's Birth Date	(0010,0030)	2	Entered on Patient card, Date Of Birth field, or filled-in from worklist.
Patient's Sex	(0010,0040)	2	Entered on Patient card, Sex selection, or filled-in from worklist.
Referenced Patient Sequence	(0008,1120)	3	Not used.
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
Patient's Birth Time	(0010,0032)	3	Not used.
Other Patient IDs	(0010,1000)	3	Entered on Patient card, Other Ids field, or filled-in from worklist.
Other Patient Names	(0010,1001)	3	Entered on Patient card, Other Names field, or filled-in from worklist.
Ethnic Group	(0010,2160)	3	Entered on Patient card, Ethnic Group field, or filled-in from worklist.
Patient Comments	(0010,4000)	3	Entered on Patient card, Comments field, or filled-in from worklist.

3.5.1.2 GENIE Acquisition Patient Module

This section specifies the Attributes of the patient that describe and identify the patient who is the subject of a diagnostic Study. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

TABLE 3.5-2  
GENIE ACQUISITION PATIENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Patient Flags	(0009,xx41)	3	Defines patient information.
Patient Creation Date	(0009,xx42)	3	Date of Patient Entity creation.
Patient Creation Time	(0009,xx43)	3	Time of Patient Entity creation.



3.5.2 Common Study Entity Modules

The following Study IE Modules are common to all Composite Image IODs which reference the Study IE. These Module contain Attributes of the patient and study that are needed for diagnostic interpretation of the image.

3.5.2.1 General Study Module

This section specifies the Attributes which describe and identify the study performed upon the patient.

TABLE 3.5-3  
GENERAL STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Study Instance UID	(0020,000D)	1	Internally generated, or filled-in from worklist.
Study Date	(0008,0020)	2	Creation date of study entity (yyyymmdd).
Study Time	(0008,0030)	2	Creation time of study entity (hhmmss).
Referring Physician's Name	(0008,0090)	2	Entered on Study card, Referring Phys field, or filled-in from worklist.
Study ID	(0020,0010)	2	Entered on Study card, Processing Tag field.
Accession Number	(0008,0050)	2	Entered on Study card, Accession Number field, or filled-in from worklist.
Study Description	(0008,1030)	3	Entered on To Do card, Study Name field.
Physician(s) of Record	(0008,1048)	3	Not used.
Name of Physician(s) Reading Study	(0008,1060)	3	Entered on Study card, Reading Phys field, or filled-in from worklist.
Referenced Study Sequence	(0008,1110)	3	Not used.
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
Procedure Code Sequence	(0008,1032)	3	Not used.
>Code Value	(0008,0100)	1C	Not used.
>Coding Scheme Designator	(0008,0102)	1C	Not used.
>Coding Scheme Version	(0008,0104)	1C	Not used.

3.5.2.2 Patient Study Module

This section defines Attributes that provide information about the Patient at the time the Study was performed.

TABLE 3.5-4  
PATIENTS STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Admitting Diagnoses Description	(0008,1080)	3	Displayed in Worklist view, filled-in from worklist.
Patient's Age	(0010,1010)	3	Entered on Patient card, Age field, or filled-in from worklist.
Patient's Size	(0010,1020)	3	Entered on Patient card, Height field, or filled-in from worklist.
Patient's Weight	(0010,1030)	3	Entered on Patient card, Weight field, or filled-in from worklist.
Occupation	(0010,2180)	3	Entered on Patient card, Occupation field, or filled-in from worklist.

Additional Patient's History	(0010,21B0)	3	Entered on Patient card, History field, or filled-in from worklist.
------------------------------	-------------	---	---

**3.5.2.3 GENIE Acquisition Study Module**

This section specifies the Attributes which describe and identify the Study performed upon the Patient. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

**TABLE 3.5-5  
GENIE ACQUISITION STUDY MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Study Flags	(0009,xx11)	3	Defines study information.
Study Type	(0009,xx12)	3	Defines type of study.
Study Comments	(0013,xx26)	3	User-defined additional information about the study.

**3.5.3 Common Series Entity Modules**

The following Series IE Modules are common to all Composite Image IODs which reference the Series IE.

**3.5.3.1 General Series Module**

This section specifies the Attributes which identify and describe general information about the Series within a Study.

**TABLE 3.5-6  
GENERAL SERIES MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Modality	(0008,0060)	1	Internally set to "NM".
Series Instance UID	(0020,000E)	1	Internally generated.
Series Number	(0020,0011)	2	Internally generated.
Laterality	(0020,0060)	2C	Entered on Image card; sent if present.
Series Date	(0008,0021)	3	Date of acquisition completion.
Series Time	(0008,0031)	3	Time of acquisition completion.
Performing Physicians' Name	(0008,1050)	3	Entered on Study card, or filled-in from worklist.
Protocol Name	(0018,1030)	3	Entered on To Do card, Study Name field.
Series Description	(0008,103E)	3	Entered on To Do card, Series Name field.
Operators' Name	(0008,1070)	3	Not used.
Referenced Study Component Sequence	(0008,1111)	3	Not used.
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
Body Part Examined	(0018,0015)	3	Entered on Image card, Part field.

Patient Position	(0018,5100)	2C	Entered on Image card, Position selection The Defined Terms are: HFP = Head First-Prone HFS = Head First-Supine HFDR = Head First-Decubitus Right HFDL = Head First-Decubitus Left FFDR = Feet First-Decubitus Right FFDL = Feet First-Decubitus Left FFP = Feet First-Prone FFS = Feet First-Supine
Smallest Pixel Value in Series	(0028,0108)	3	Not used (see Image Pixel module).
Largest Pixel Value in Series	(0028,0109)	3	Not used (see Image Pixel module).
Request Attributes Sequence	(0040,0275)	3	Attributes from the ISR.
> Requested Procedure ID	(0040,4001)	1C	Entered on Study Card or filled-in from worklist.
> Scheduled Procedure Step ID	(0040,0009)	1C	Entered on Study Card or filled-in from worklist.
> Scheduled Procedure Step Description	(0040,0007)	3	Filled-in from worklist.
>Scheduled Action Item Code Sequence	(0040,0008)	3	Not used.
>>Code Value	(0008,0100)	1C	Not used.
>>Coding Scheme Designator	(0008,0102)	1C	Not used.
>>Coding Scheme Version	(0008,0104)	1C	Not used.
Performed Procedure Step ID	(0040,0253)	3	Not used.
Performed Procedure Step Start Date	(0040,0244)	3	Not used.
Performed Procedure Step Start Time	(0040,0245)	3	Not used.
Performed Procedure Step Description	(0040,0254)	3	Not used.
Performed Action Item Sequence	(0040,0260)	3	Not used.
>Code Value	(0008,0100)	1C	Not used.
>Coding Scheme Designator	(0008,0102)	1C	Not used.
>Coding Scheme Version	(0008,0104)	1C	Not used.

3.5.3.2 GENIE Acquisition Series Module

This section specifies the Attributes which identify and describe general information about the Series within a Study. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

TABLE 3.5-7  
GENIE ACQUISITION SERIES MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Series Flags	(0009,xx21)	3	Defines series information.
User Orientation	(0009,xx22)	3	User specified patient orientation.
Initiation Type	(0009,xx23)	3	Acquisition initiation type. The Defined Terms are: 0 = started on count rate 1 = started after time delay 2 = started manually
Initiation Delay	(0009,xx24)	3	Acquisition start delay time.
Initiation Count Rate	(0009,xx25)	3	Acquisition start count rate
Number Energy Sets	(0009,xx26)	3	Number of energy sets (windows).
Number Detectors	(0009,xx27)	3	Number of detectors.
Series Comments	(0009,xx2C)	3	User-defined additional information about the series.
Distance Prescribed	(0009,xx2E)	3	User prescribed whole body scanning distance.

Series Type	(0011,xx0A)	3	Defines type of series. The Defined Terms are: 0 = static 1 = whole body 3 = multi-gated 6 = dynamic 9 = tomographic
Effective Series Duration	(0011,xx0B)	3	Duration of series acquisition.
Number Beats	(0011,xx0C)	3	Number of physiological triggers during acquisition.

**3.5.4 Common Frame Of Reference Entity Modules**

The following Frame of Reference IE Module is common to all Composite Image IODs which reference the Frame of Reference IE.

**3.5.4.1 Frame Of Reference Module**

This section specifies the Attributes necessary to uniquely identify a Frame Of Reference which insures the spatial relationship of Images within a Series. It also allows Images across multiple Series to share the same Frame Of Reference. This Frame Of Reference (or coordinate system) shall be constant for all Images related to a specific Frame Of Reference.

GENIE Acquisition groups spatially and/or temporally related Images in the same Series. Although multiple Series in a Study may be spatially and/or temporally related, this implementation does not convey this information.

**TABLE 3.5-8  
FRAME OF REFERENCE MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Frame of Reference UID	(0020,0052)	1	See 3.5.4.1.1.1 for further explanation.
Position Reference Indicator	(0020,1040)	2	See 3.5.4.1.1.2 for further explanation.

**3.5.4.1.1 Frame Of Reference Attribute Descriptions**

**3.5.4.1.1.1 Frame Of Reference UID**

The Frame Of Reference UID is set to a value unique to every Series. This is done because images of a given series are assumed to be spatially and/or temporally related.

**3.5.4.1.1.2 Position Reference Indicator**

The Position Reference Indicator (0020,1040) is used to specify the part of the patient’s anatomy which was used as an anatomical reference point associated with a specific Frame of Reference UID. The value of the Position Reference Indicator is entered on the Image card, “Ref:” field.

**3.5.5 Common Equipment Entity Modules**

The following Equipment IE Module is common to all Composite Image IODs which reference the Equipment IE.

**3.5.5.1 General Equipment Module**

This section specifies the Attributes which identify and describe the piece of equipment which produced a Series of Images.

**TABLE 3.5-9  
GENERAL EQUIPMENT MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Manufacturer	(0008,0070)	2	Set to "GE MEDICAL SYSTEMS".
Institution Name	(0008,0080)	3	Set to value displayed on user interface banner.
Institution Address	(0008,0081)	3	Not used.
Station Name	(0008,1010)	3	Set to the name of station data acquired on.
Institutional Department Name	(0008,1040)	3	Not used.
Manufacturer's Model Name	(0008,1090)	3	Set to system type data acquired on.
Device Serial Number	(0018,1000)	3	Set to serial number data acquired on.
Software Versions	(0018,1020)	3	Set to GENIE Acquisition software version.
Spatial Resolution	(0018,1050)	3	Not used.
Date of Last Calibration	(0018,1200)	3	Not used.
Time of Last Calibration	(0018,1201)	3	Not used.
Pixel Padding Value	(0028,0120)	3	Not used.

**3.5.6 Common Image Entity Modules**

The following Image IE Modules are common to all Composite Image IODs which reference the Image IE.

**3.5.6.1 General Image Module**

This section specifies the Attributes which identify and describe an image within a particular series.

**TABLE 3.5-10  
GENERAL IMAGE MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Image Number	(0020,0013)	2	Internally generated.
Patient Orientation	(0020,0020)	2C	Not used.
Content Date	(0008,0023)	2C	Date of acquisition completion (yyyymmdd).
Content Time	(0008,0033)	2C	Time of acquisition completion (hhmmss).
Image Type	(0008,0008)	3	See NM Image module.
Acquisition Number	(0020,0012)	3	Not used.
Acquisition Date	(0008,0022)	3	Date of acquisition completion.
Acquisition Time	(0008,0032)	3	Time of acquisition completion.
Acquisition Datetime	(0008,002A)	3	Not used.

Referenced Image Sequence	(0008,1140)	3	Images from the same series acquired by the same detector
>Referenced SOP Class UID	(0008,1150)	1C	Set to "1.2.840.10008.5.1.4.1.1.20", Nuclear Medicine Image Storage SOP Class UID.
>Referenced SOP Instance UID	(0008,1155)	1C	Internally generated.
>Referenced Frame Number	(0008,1160)	3	Not used.
Derivation Description	(0008,2111)	3	Not used.
Source Image Sequence	(0008,2112)	3	Not used..
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
>Referenced Frame Number	(0008,1160)	3	Not used.
Images in Acquisition	(0020,1002)	3	Number of images in the series
Image Comments	(0020,4000)	3	Not used.
Quality Control Image	(0020,4000)	3	Not used.
Burned In Annotation	(0028,0301)	3	Not used.
Lossy Image Compression	(0028,2110)	3	Not used. Images are never compressed.
Lossy Image Compression Ratio	(0028,2112)	3	Not used.

3.5.6.2 GENIE Acquisition Image Module

This section specifies the Attributes which identify and describe an image within a particular series. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

TABLE 3.5-11  
GENIE ACQUISITION IMAGE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Radio Nuclide Name	(0011,xx0D)	3	Name of radionuclide used.
Dataset Name	(0011,xx12)	3	Name of imageset in Starlink or Xpert format.
Dataset Type	(0011,xx13)	3	Defines type of dataset. The Defined Terms are: 0 = static 2 = whole body 8 = dynamic 11 = multi-gated 12 = tomographic planar
Detector Number	(0011,xx15)	3	Detector number image was acquired by. This field is not valid for data from more than one detector.
Energy Number	(0011,xx16)	3	Energy set number.
RR Interval Window Number	(0011,xx17)	3	R-R interval number (TIAR number).
MG Bin Number	(0011,xx18)	3	Multi-gated interval number. This field is not valid for data from more than one interval.
Radius Of Rotation	(0011,xx19)	3	Distance to the center of detector rotation.
Detector Count Zone	(0011,xx1A)	3	FOV zone for count-based acquisition termination criteria. The Defined Terms are: 0 = none specified 1 = total (all) counts 2 = counts in energy set 3 = counts inside an ROI 4 = counts outside an ROI
Num Energy Windows	(0011,xx1B)	3	Number of energy windows in energy set.

Image Orientation	(0011,xx1F)	3	Orientation of the image. The Defined Terms are: 0 = no rotation, no mirroring 1 = no rotation, mirrored
Table Orientation	(0011,xx26)	3	Orientation of the table for whole body acquisition. The Defined Terms are: 0 = direction in/out 1 = direction left/right
ROI Top Left	(0011,xx27)	3	Acquisition count zone ROI, top left coordinate.
ROI Bottom Right	(0011,xx28)	3	Acquisition count zone ROI, bottom right coordinate.
Energy Correct Name	(0011,xx33)	3	Name of applied energy correction.
Spatial Correct Name	(0011,xx34)	3	Name of applied spatial correction.
Tuning Calib Name	(0011,xx35)	3	Name of applied tuning calibration data.
Uniformity Correct Name	(0011,xx36)	3	Name of associated uniformity correction.
Acquisition Specific Correct Name	(0011,xx37)	3	Name(s) of associated acquisition specific correction(s).
Dataset Flags	(0011,xx3F)	3	Defines dataset information.
Period	(0011,xx55)	3	Set to 1.0.
Elapsed Time	(0011,xx56)	3	Set to 1.0.
Digital FOV	(0011,xx10)	3	Field-of-view size.

3.5.6.3 Image Pixel Module

This section specifies the Attributes that describe the pixel data of the image.

TABLE 3.5-12  
IMAGE PIXEL MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Samples per Pixel	(0028,0002)	1	See NM Image Pixel module.
Photometric Interpretation	(0028,0004)	1	See NM Image Pixel module.
Rows	(0028,0010)	1	Will be one of the following values: 64, 128, 256, 512, 1024.
Columns	(0028,0011)	1	Will be one of the following values: 64, 128, 256, 512.
Bits Allocated	(0028,0100)	1	See NM Image Pixel module.
Bits Stored	(0028,0101)	1	See NM Image Pixel module.
High Bit	(0028,0102)	1	See NM Image Pixel module.
Pixel Representation	(0028,0103)	1	Set to 0001H (2's complement).
Pixel Data	(7FE0,0010)	1	Acquired NM count data.
Planar Configuration	(0028,0006)	1C	Not used. Attribute not required since Samples per Pixel (0028,0002) is always 1.
Pixel Aspect Ratio	(0028,0034)	1C	Not used. Attribute not required since aspect ratio is always 1\1.
Smallest Image Pixel Value	(0028,0106)	3	Set to minimum pixel value in image.
Largest Image Pixel Value	(0028,0107)	3	Set to maximum pixel value in image.
Red Palette Color Lookup Table Descriptor	(0028,1101)	1C	Not used.
Green Palette Color Lookup Table Descriptor	(0028,1102)	1C	Not used.
Blue Palette Color Lookup Table Descriptor	(0028,1103)	1C	Not used.
Red Palette Color Lookup Table Data	(0028,1201)	1C	Not used.
Green Palette Color Lookup Table Data	(0028,1202)	1C	Not used.
Blue Palette Color Lookup Table Data	(0028,1203)	1C	Not used.

3.5.6.4 GENIE Acquisition Image Pixel Module

This section specifies the Attributes that describe the pixel data of the image. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

TABLE 3.5-13  
GENIE ACQUISITION IMAGE PIXEL MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Byte Order	(0011,xx38)	3	Defines pixel data byte order. The Defined Terms are: = little endian 66 = big endian
Picture Format	(0011,xx3A)	3	Set to 5 (GENIE IAP image format).
Pixel Scale	(0011,xx3B)	3	Set to 1.0.
Pixel Offset	(0011,xx3C)	3	Set to 0.0.
Threshold Center	(0011,xx44)	3	Set to 2048.0.
Threshold Width	(0011,xx45)	3	Set to 4096.0.
Interpolation Type	(0011,xx38)	3	Set to 2.

3.5.6.5 Multi-Frame Module

This section specifies the Attributes of a Multi-frame pixel data Image.

TABLE 3.5-14  
MULTI-FRAME MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Number of Frames	(0028,0008)	1	Set to total number of frames in image.
Frame Increment Pointer	(0028,0009)	1	See 3.5.6.5.1.1 for further explanation.

3.5.6.5.1 Multi-Frame Attribute Descriptions

3.5.6.5.1.1 Frame Increment Pointer

See the NM Multi-frame Module for further information.



3.5.7 General Modules

The SOP Common Module is mandatory for all DICOM IODs.

3.5.7.1 SOP Common Module

This section defines the Attributes which are required for proper functioning and identification of the associated SOP Instances. They do not specify any semantics about the Real-World Object represented by the IOD.

TABLE 3.5-15  
SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
SOP Class UID	(0008,0016)	1	Set to "1.2.840.10008.5.1.4.1.1.20", Nuclear Medicine Image Storage SOP Class UID.
SOP Instance UID	(0008,0018)	1	Internally generated.
Specific Character Set	(0008,0005)	1C	"ISO_IR 100".
Instance Creation Date	(0008,0012)	3	Date of instance creation.
Instance Creation Time	(0008,0013)	3	Time of instance creation.
Instance Creator UID	(0008,0014)	3	Not used.

3.5.8 Nuclear Medicine Modules

This Section describes Nuclear Medicine Series, and Image Modules. These Modules contain Attributes that are specific to the NM Image IOD.

Note that more than one SOP Instance can be used to encode a single NM acquisition. For example, for Multi-gated Tomographic acquisitions, the data for each gate is sent in a separate SOP Instance as a separate Multi-gated Tomographic image. It is valid for the receiving AE to recombine the SOP Instances, per the structure of the NM IOD, to form a new SOP Instance.

3.5.8.1 NM/PET Patient Orientation Module

This section specifies the Attributes that describe the NM Series.

TABLE 3.5-16  
NM/PET PATIENT ORIENTATION MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Patient Orientation Code Sequence	(0054,0410)	2	Not used.
> Code Value	(0008,0100)	1C	Not used.
> Coding Scheme Designator	(0008,0102)	1C	Not used.
> Code Meaning	(0008,0104)	3	Not used.
> Patient Orientation Modifier Code Sequence	(0054,0412)	2C	Not used.
>> Code value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.
Patient Gantry Relationship Code Sequence	(0054,0414)	2	Not used.
> Code Value	(0008,0100)	1C	Not used.

> Coding Scheme Designator	(0008,0102)	1C	Not used..
> Code Meaning	(0008,0104)	3	Not used.

**3.5.8.2 NM Image Pixel Module**

This section specifies the Attributes that describe the pixel data of a NM image.

**TABLE 3.5-17**  
**NM IMAGE PIXEL MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Samples per Pixel	(0028,0002)	1	Set to 1.
Photometric Interpretation	(0028,0004)	1	Set to Enumerated Value MONOCHROME2.
Bits Allocated	(0028,0100)	1	Set to 16.
Bits Stored	(0028,0101)	1	Set to 16.
High Bit	(0028,0102)	1	Set to 15.
Pixel Spacing	(0028,0030)	2	Set to size of pixels in image.

**3.5.8.3 NM Multi-frame Module**

This section specifies the Attributes of a NM Multi-frame Image. This module is always included in a NM SOP instance, even if there is only one frame in the image.

**TABLE 3.5-18**  
**NM MULTI-FRAME MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Frame Increment Pointer	(0028,0009)	1	See 3.5.8.3.1.1 for further specialization.
Energy Window Vector	(0054,0010)	1C	Defines energy window to which each frame belongs.
Number of Energy Windows	(0054,0011)	1	Set to number of energy windows in SOP Instance.
Detector Vector	(0054,0020)	1C	Defines detector to which each frame belongs.
Number of Detectors	(0054,0021)	1	Set to number of detectors in SOP Instance.
Phase Vector	(0054,0030)	1C	Defines phases to which each frame belongs.
Number of Phases	(0054,0031)	1C	Set to number of phase in SOP Instance.
Rotation Vector	(0054,0050)	1C	All indices set to 1.
Number of Rotations	(0054,0051)	1C	Set to 1.
R-R Interval Vector	(0054,0060)	1C	All indices set to 1.
Number of R-R Intervals	(0054,0061)	1C	Set to 1.
Time Slot Vector	(0054,0070)	1C	Defines time slot, within cardiac cycle, to which each frame belongs.
Number of Time Slots	(0054,0071)	1C	Set to number of time slots in SOP Instance.
Slice Vector	(0054,0080)	1C	All indices set to 1.
Number of Slices	(0054,0081)	1C	Set to 1.
Angular View Vector	(0054,0090)	1C	Defines angular view number to which each frame belongs.
Time Slice Vector	(0054,0100)	1C	Defines frame numbers within each phase.

3.5.8.3.1 NM Multi-Frame Attribute Descriptions

3.5.8.3.1.1 Frame Increment Pointer

The Frame Increment Pointer (0028,0009) defines which frame index vectors are present in the NM Multi-frame Module. Not all frame index vectors are present for each image type. The Frame Increment Pointer is supported per the DICOM specification for all image types defined in Table 3.5-19.

TABLE 3.5-19  
ENUMERATED VALUES FOR FRAME INCREMENT POINTER

Image Type (0008,0008), Value 3	Frame Increment Pointer (0028,0009)
STATIC or WHOLE BODY	0054H 0010H \ 0054H 0020H Sequencing is by Energy Window Vector (0054,0010), Detector Vector (0054,0020).
DYNAMIC	0054H 0010H \ 0054H 0020H \ 0054H 0030H \ 0054H 0100H Sequencing is by Energy Window Vector (0054,0010), Detector Vector (0054,0020), Phase Vector (0054,0030), Time Slice Vector (0054,0100)
GATED	0054H 0010H \ 0054H 0020H \ 0054H 0060H \ 0054H 0070H Sequencing is by Energy Window Vector (0054,0010), Detector Vector (0054,0020), R-R Interval Vector(0054,0060), Time Slot Vector (0054,0070)
TOMO	0054H 0010H \ 0054H 0020H \ 0054H 0050H \ 0054H 0090H Sequencing is by Energy Window Vector (0054,0010), Detector Vector (0054,0020), Rotation Vector (0054,0050), Angular View Vector (0054,0090)
GATED TOMO	0054H 0010H \ 0054H 0020H \ 0054H 0050H \ 0054H 0060H \ 0054H 0070H \ 0054H 0090H Sequencing is by Energy Window Vector (0054,0010), Detector Vector (0054,0020), Rotation Vector (0054,0050), R-R Interval Vector (0054,0060), Time Slot Vector (0054,0070), Angular View Vector (0054,0090).

3.5.8.4 NM Image Module

This section contains the Attributes that describe Nuclear Medicine Images.

TABLE 3.5-20  
NM IMAGE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Image Type	(0008,0008)	1	See 3.5.8.4.1.1 for specialization.
Image ID	(0054,0400)	3	Set to name of imageset.
Lossy Image Compression	(0028,2110)	1C	Not used. Images never compressed.
Counts Accumulated	(0018,0070)	2	Set to number of counts in imageset.
Acquisition Termination Condition	(0018,0071)	3	Defined Terms used: CNTS = count limit reached DENS = count limit reached within ROI MANU = manual TIME = time limit reached TRIG = number of beats limit reached
Table Height	(0018,1130)	3	Height of table above floor at acquisition start. Sent if system is capable of measuring this value.
Table Traverse	(0018,1131)	3	Table longitudinal position at acquisition start. Sent if system is capable of measuring this value.
Actual Frame Duration	(0018,1242)	1C	Duration of each frame in imageset.
Count Rate	(0018,1243)	3	Maximum count rate during image acquisition.

Processing Function	(0018,5020)	3	Not used.
Corrected Image	(0028,0051)	3	Defined Terms used: NRGY = energy corrected LIN = linearity corrected UNIF = uniformity corrected COR = center of rotation corrected NCO = non-circular orbit corrected DECY = decay corrected
Whole Body Technique	(0018,1301)	3	Enumerated Values used: 1PS = one pass
Scan Velocity	(0018,1300)	2C	Whole body scan speed
Scan Length	(0018,1302)	2C	Whole body scan length
Referenced Overlay Sequence	(0008,1130)	3	Not used.
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
Referenced Curve Sequence	(0008,1145)	3	Not used.
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
Trigger Source or Type	(0018,1061)	3	Defined Terms used: EKG
Anatomic Region Sequence	(0008,2218)	3	Not used.
> Code Value	(0008,0100)	1C	Not used.
> Coding Scheme Designator	(0008,0102)	1C	Not used.
> Code Meaning	(0008,0104)	3	Not used.
> Anatomic Region Modifier Sequence	(0008,2220)	3	Not used.
>> Code Value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.
Primary Anatomic Structure Sequence	(0008,2228)	3	Not used.
> Code Value	(0008,0100)	1C	Not used.
> Coding Scheme Designator	(0008,0102)	1C	Not used.
> Code Meaning	(0008,0104)	3	Not used.
> Primary Anatomic Structure Modifier Sequence	(0008,2230)	3	Not used.
>> Code Value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.

3.5.8.4.1 NM Image Module Attribute Descriptions

3.5.8.4.1.1 Image Type

The following Image Type (0008,0008) values are sent:

Value 1 shall have the following Enumerated Value:

ORIGINAL identifies an Original Image

Value 2 shall have the following Enumerated Value:

PRIMARY identifies a Primary Image

Value 3 shall have the following Enumerated Values:

STATIC identifies a Static Image

DYNAMIC identifies a Dynamic Image

GATED identifies a Multi-gated Image  
 WHOLE BODY identifies a Whole Body Image  
 TOMO identifies a Tomographic Image  
 GATED TOMO identifies a Multi-gated Tomographic Image  
 Value 4 shall have the following Enumerated Values:  
 EMISSION transmission source NOT active during image acquisition  
 TRANSMISSION transmission source active during image acquisition

**3.5.8.5 NM Isotope Module**

This section contains Attributes that describe the isotope administered for the acquisition.

**TABLE 3.5-21**  
**NM ISOTOPE MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Energy Window Information Sequence	(0054,0012)	2	Energy window information.
> Energy Window Name	(0054,0018)	3	Entered on Energy/Set N card, Emission Name and/or Transmission Name field.
>Energy Window Range Sequence	(0054,0013)	3	Sequence describing window energy limits.
>> Energy Window Lower Limit	(0054,0014)	3	Lower energy limit in KeV.
>> Energy Window Upper Limit	(0054,0015)	3	Upper energy limit in KeV.
Radiopharmaceutical Information Sequence	(0054,0016)	2	Information on radiopharmaceutical(s) used.
> Radionuclide Code Sequence	(0054,0300)	2C	Not used (Zero length).
>> Code Value	(0008,0100)	1C	Entered on Energy/Isotope card, Isotope field. See 3.5.8.5.1 for specialization..
>> Coding Scheme Designator	(0008,0102)	1C	See 3.5.8.5.1 for specialization.
>> Code Meaning	(0008,0104)	3	See 3.5.8.5.1 for specialization.
> Radiopharmaceutical Route	(0018,1070)	3	Not used.
> Administration Route Code Sequence	(0054,0302)	3	Not used.
>> Code Value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.
> Radiopharmaceutical Volume	(0018,1071)	3	Entered on Energy/Isotope card, Nuclide Vol field.
> Radiopharmaceutical Start Time	(0018,1072)	3	Not used.
> Radiopharmaceutical Stop Time	(0018,1073)	3	Not used.
> Radionuclide Total Dose	(0018,1074)	3	Entered on Energy/Isotope card, Total Dose field.
> Calibration Data Sequence	(0054,0306)	3	Dose information.
>> Energy Window Number	(0054,0308)	1C	Set to 1.
>> Syringe Counts	(0018,1045)	3	Entered on Energy/Isotope card, Dose field.
>> Residual Syringe Counts	(0054,0017)	3	Entered on Energy/Isotope card, Residual Dose field.
> Radiopharmaceutical	(0018,0031)	3	Entered on Energy/Isotope card, Pharm field.
> Radiopharmaceutical Code Sequence	(0054,0304)	3	Not used.
>> Code Value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.
Intervention Drug Information Sequence	(0018,0026)	3	Not used.
>Intervention Drug Name	(0018,0034)	3	Not used.
>Intervention Drug Code Sequence	(0018,0029)	3	Not used.

>> Code Value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.
> Administration Route Code Sequence	(0054,0302)	3	Not used.
>> Code Value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.
>Intervention Drug Start Time	(0018,0035)	3	Not used.
>Intervention Drug Stop Time	(0018,0027)	3	Not used.
>Intervention Drug Dose	(0018,0028)	3	Not used.

**3.5.8.5.1 Radionuclide Code Sequence**

The Coding Scheme Designator (0008,0102) for the Radionuclide Code Sequence (0054,0300) shall be “99SDM” representing the SNOMED DICOM Microglossary.

The Code Value (0008,0100) is entered by the user. It can be any of the values from the Code Value or Alternative GE Value columns shown in the table below.

The Code Meaning (0008,0104) depends on the Code Value (0008,0100) and will take one of the following enumerated values:

<b>Code Meaning (0008,0104)</b>	<b>Code Value (0008,0100)</b>	<b>Alternative GE Value</b>
^18^Fluorine	C-111A1	F118
^123^Iodine	C-114A4	I123
^125^Iodine	C-114A6	I125
^131^Iodine	C-114B1	I131
^133^Barium	C-122A5	Ba133
^67^Gallium	C-131A2	Ga67
^201^Thallium	C-138A9	Tl201
^57^Cobalt	C-144A3	Co57
^111^Indium	C-145A4	In111
^99m^Technetium	C-163A8	Tc99m
^133^Xenon	C-172A8	Xe133
^85^Krypton	C-173A7	Kr85
^153^Gadolinium	C-178A8	Gd153
Not sent	Other	

3.5.8.6 GENIE Acquisition Isotope Module

This section contains Attributes that describe the isotope administered for the acquisition. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

TABLE 3.5-22  
GENIE ACQUISITION ISOTOPE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Energy Offset	(0011,xx1C)	3	Energy window offset as a percentage of the energy peak.
Energy Range	(0011,xx1D)	3	Defines X-series detector energy range. The Defined Terms are: 0 = low energy range 1 = high energy range
AutoTrack Peak	(0013,xx16)	3	Optima AutoTrack energy peak.
AutoTrack Width	(0013,xx17)	3	Optima AutoTrack energy width.

3.5.8.7 NM Detector Module

This section contains IOD Attributes that describe Nuclear Medicine Detectors used to produce an image.

TABLE 3.5-23  
NM DETECTOR MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Detector Information Sequence	(0054,0022)	2	Detector information.
> Collimator/Grid Name	(0018,1180)	3	Name of collimator used on this detector.
> Collimator Type	(0018,1181)	2C	Which Defined Terms used: PARA = Parallel PINH = Pinhole FANB = Fan-beam CONE = Cone-beam SLNT = Slant hole ASTG = Astigmatic DIVG = Diverging NONE = No collimator UNKN = Unknown
> Field of View Shape	(0018,1147)	3	Which Defined Terms used: RECTANGLE ROUND HEXAGONAL
> Field of View Dimension(s)	(0018,1149)	3	Dimensions of the field of view.
> Focal Distance	(0018,1182)	2C	Focal distance.
> X Focus Center	(0018,1183)	3	Center point of the focus position.
> Y Focus Center	(0018,1184)	3	Center point of the focus position.
> Zoom Center	(0028,0032)	3	Image center offset from field of view center.
> Zoom Factor	(0028,0031)	3	Zoom factor, typical range: 1.00 to 4.00.
> Center of Rotation Offset	(0018,1145)	3	Offset between detector center and mechanical center positions.
> Gantry/Detector Tilt	(0018,1120)	3	Detector tilt position.
> Distance Source to Detector	(0018,1110)	2C	Distance between transmission source and detector during transmission scanning.

> Start Angle	(0054,0200)	3	Not used.
> Radial Position	(0018,1142)	3	Detector radial position at start of acquisition.
> Image Orientation (Patient)	(0020,0037)	2C	Set to 1.0\0.0\0.0\0.0\0.0\1.0.
> Image Position (Patient)	(0020,0032)	2C	Set to 0.0\0.0\0.0.
> View Code Sequence	(0054,0220)	3	Not used.
>> Code Value	(0008,0100)	1C	Not used.
>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>> Code Meaning	(0008,0104)	3	Not used.
>> View Angulation Modifier Code Sequence	(0054,0222)	2C	Not used.
>>> Code value	(0008,0100)	1C	Not used.
>>> Coding Scheme Designator	(0008,0102)	1C	Not used.
>>> Code Meaning	(0008,0104)	3	Not used.

**3.5.8.8 GENIE Acquisition Detector Module**

This section contains Attributes that describe Nuclear Medicine Detectors used to produce an image. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

**TABLE 3.5-24  
GENIE ACQUISITION DETECTOR MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Use FOV Mask	(0011,xx23)	3	Whether FOV mask used during image acquisition. The Defined Terms are: 0 = no mask used 1 = FOV mask used
FOV Mask Y Cutoff Distance	(0011,xx24)	3	Hexagonal FOV mask Y cutoff angle.
FOV Mask Cutoff Angle	(0011,xx25)	3	Hexagonal FOV mask cutoff angle.
FOV Shape	(0011,xx3E)	3	GEMS NM system detector type. The Defined Terms are: 1 = AC400 6 = Optima, MYOCAM 7 = MAXXUS 8 = Millennium MPS, UNICAM 9 = Millennium MPR, TOMOCAM 10 = Millennium MG, MT, MC, MAGICAM
Transmission Scan Time	(0013,xx18)	3	Attenuation correction transmission scan duration.
Transmission Mask Width	(0013,xx19)	3	Attenuation correction transmission scan mask width.
Copper Attenuator Thickness	(0013,xx1A)	3	Thickness of transmission scan copper attenuator.

**3.5.8.9 NM TOMO Acquisition Module**

This section contains Attributes that describe Rotation information of a tomographic image performed on the patient. This module is present when the Image Type (0008,0008) Value 3, is equal to TOMO or GATED TOMO.

**TABLE 3.5-25  
NM TOMO ACQUISITION MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Rotation Information Sequence	(0054,0052)	2	Provides TOMO rotation information.



> Start Angle	(0054,0200)	1C	Trailing detector start angle at start of acquisition.
> Angular Step	(0018,1144)	1C	Incremental rotational angle change per view.
> Rotation Direction	(0018,1140)	1C	Direction of rotation.
> Scan Arc	(0018,1143)	1C	Total rotation angle.
> Actual Frame Duration	(0018,1242)	1C	Duration of a view.
> Radial Position	(0018,1142)	3	Detector radial position at start of acquisition.
> Distance Source to Detector	(0018,1110)	2C	Distance between transmission source and detector during transmission scanning.
> Number of Frames in Rotation	(0054,0053)	1C	Number of tomographic views acquired.
> Table Traverse	(0018,1131)	3	Table longitudinal position at acquisition start.
> Table Height	(0018,1130)	3	Height of table above floor at acquisition start.
Type of Detector Motion	(0054,0202)	3	Enumerated Values used: STEP AND SHOOT = Interrupted motion, acquire only while stationary. CONTINUOUS = Gantry motion and acquisition are simultaneous and continuous. ACQ DURING STEP = Interrupted motion, acquisition is continuous.

3.5.8.10 GENIE Acquisition TOMO Acquisition Module

This section contains Attributes that describe Rotation information of a tomographic acquisition image performed on the patient. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

TABLE 3.5-26  
GENIE ACQUISITION TOMO ACQUISITION MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Gantry Locus Type	(0009,xx35)	3	Locus type of gantry motion during acquisition. The Defined Terms are: 0 = circular 1 = elliptical
Tomo View Offset	(0013,xx1E)	3	Table of offsets from COR during acquisition.

3.5.8.11 NM Multi-gated Acquisition Module

This section contains Attributes that describe a multi-gated acquisition performed on the patient. This refers to frames acquired while the patient is connected to a gating device. This module is present when the Image Type (0008,0008) Value 3, is equal to GATED or GATED TOMO.

TABLE 3.5-27  
NM MULTI-GATED ACQUISITION MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Beat Rejection Flag	(0018,1080)	3	Whether a bad beat rejection algorithm used. Enumerated values: Y = bad beat rejection algorithm used N = bad beat rejection algorithm NOT used
PVC Rejection	(0018,1085)	3	Set to "AMGB buffered beats with single acceptance window".

Skip Beats	(0018,1086)	3	Set to 1.
Heart Rate	(0018,1088)	3	Average heart rate during acquisition.
Gated Information Sequence	(0054,0062)	2C	One sequence item present.
> Trigger Time	(0018,1060)	3	Not used.
> Framing Type	(0018,1064)	3	Not used.
> Data Information Sequence	(0054,0063)	2C	One sequence item present.
>> Frame Time	(0018,1063)	1C	Gated frame duration in the imageset.
>> Nominal Interval	(0018,1062)	3	Not used.
>> Low R-R Value	(0018,1081)	3	Minimum R-R interval value accepted.
>> High R-R Value	(0018,1082)	3	Maximum R-R interval value accepted.
>> Intervals Acquired	(0018,1083)	3	Number of accepted intervals.
>> Intervals Rejected	(0018,1084)	3	Number of rejected intervals.
>> Time Slot Information Sequence	(0054,0072)	2C	Not used.
>>> Time Slot Time	(0054,0073)	3	Not used.

**3.5.8.12 GENIE Acquisition Multi-gated Acquisition Module**

This section contains Attributes that describe a multi-gated acquisition performed on the patient. This refers to frames acquired while the patient is connected to a gating device. This Module contains *private* Attributes that convey information not contained in similar DICOM Standard v3.0 Module(s).

**TABLE 3.5-28**  
**GENIE ACQUISITION MULTI-GATED ACQUISITION MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Starting Heart Rate	(0009,xx37)	3	Heart rate at start of acquisition.
Track Beat Average	(0009,xx2D)	3	Whether heart rate tracking used during acquisition.
RR Window Width	(0009,xx38)	3	Width of RR acceptance window as percentage of rate.
RR Window Offset	(0009,xx39)	3	Offset of RR acceptance window as percentage of rate.
Percent Cycle Imaged	(0009,xx3A)	3	Percentage of RR cycle imaged.

**3.5.8.13 NM Phase Module**

This section contains Attributes that describe dynamic phases of a dynamic acquisition image performed on the patient. This module is present when the Image Type (0008,0008) Value 3, is equal to DYNAMIC.

**TABLE 3.5-29**  
**NM PHASE MODULE ATTRIBUTES**

Attribute Name	Tag	Type	Attribute Description
Phase Information Sequence	(0054,0032)	2C	One sequence item per dynamic phase.
> Phase Delay	(0054,0036)	1C	Set to 0.
> Actual Frame Duration	(0018,1242)	1C	Duration of all frames in this phase.
> Pause Between Frames	(0054,0038)	1C	Set to 0.
> Number of Frames in Phase	(0054,0033)	1C	Number of frames in this phase.
>Trigger Vector	(0054,0210)	3	A string of the form “T1\T2\T3\...\...”
>Number of Triggers in Phase	(0054,0211)	1C	Number of triggers in this phase

3.6 PRIVATE DATA DICTIONARY

This section provides value representation and multiplicity information for all of the Private Attributes used by this implementation. Private Attributes contained within the Information Model are described in the preceding sections.

TABLE 3.6-1  
PRIVATE CREATOR IDENTIFICATION (GEMS\_GENIE\_1)

Attribute Name	Tag	VR	VM
Private Creator Identification	(0009,0010)	LO	1
Study Flags	(0009,xx11)	SL	1
Study Type	(0009,xx12)	SL	1
Series Flags	(0009,xx21)	SL	1
User Orientation	(0009,xx22)	SH	1
Initiation Type	(0009,xx23)	SL	1
Initiation Delay	(0009,xx24)	SL	1
Initiation Count Rate	(0009,xx25)	SL	1
Number Energy Sets	(0009,xx26)	SL	1
Number Detectors	(0009,xx27)	SL	1
Series Comments	(0009,xx2C)	LO	1
Track Beat Average	(0009,xx2D)	SL	1
Distance Prescribed	(0009,xx2E)	FD	1
Gantry Locus Type	(0009,xx35)	SL	1
Starting Heart Rate	(0009,xx37)	SL	1
RR Window Width	(0009,xx38)	SL	1
RR Window Offset	(0009,xx39)	SL	1
Percent Cycle Imaged	(0009,xx3A)	SL	1
Patient Flags	(0009,xx41)	SL	1
Patient Creation Date	(0009,xx42)	DA	1
Patient Creation Time	(0009,xx43)	TM	1
Private Creator Identification	(0011,0010)	LO	1
Series Type	(0011,xx0A)	SL	1
Effective Series Duration	(0011,xx0B)	SL	1
Num Beats	(0011,xx0C)	SL	1
Radio Nuclide Name	(0011,xx0D)	LO	1
Dataset Name	(0011,xx12)	LO	1
Dataset Type	(0011,xx13)	SL	1
Detector Number	(0011,xx15)	SL	1
Energy Number	(0011,xx16)	SL	1
RR Interval Window Number	(0011,xx17)	SL	1
MG Bin Number	(0011,xx18)	SL	1
Radius Of Rotation	(0011,xx19)	FD	1
Detector Count Zone	(0011,xx1A)	SL	1
Num Energy Windows	(0011,xx1B)	SL	1
Energy Offset	(0011,xx1C)	SL	4
Energy Range	(0011,xx1D)	SL	1
Image Orientation	(0011,xx1F)	SL	1
Use FOV Mask	(0011,xx23)	SL	1
FOV Mask Y Cutoff Angle	(0011,xx24)	SL	1

FOV Mask Cutoff Angle	(0011,xx25)	SL	1
Table Orientation	(0011,xx26)	SL	1
ROI Top Left	(0011,xx27)	SL	2
ROI Bottom Right	(0011,xx28)	SL	2
Energy Correct Name	(0011,xx33)	LO	1
Spatial Correct Name	(0011,xx34)	LO	1
Tuning Calib Name	(0011,xx35)	LO	1
Uniformity Correct Name	(0011,xx36)	LO	1
Acquisition Specific Correction Name	(0011,xx37)	LT	1
Byte Order	(0011,xx38)	SL	1
Picture Format	(0011,xx3A)	SL	1
Pixel Scale	(0011,xx3B)	FD	1
Pixel Offset	(0011,xx3C)	FD	1
FOV Shape	(0011,xx3E)	SL	1
Dataset Flags	(0011,xx3F)	SL	1
Threshold Center	(0011,xx44)	FD	1
Threshold Width	(0011,xx45)	FD	1
Interpolation Type	(0011,xx46)	SL	1
Period	(0011,xx55)	FD	1
Elapsed Time	(0011,xx56)	FD	1
Private Creator Identification	(0013,0010)	LO	1
Digital FOV	(0013,xx10)	FD	2
AutoTrack Peak	(0013,xx16)	SL	1
AutoTrack Width	(0013,xx17)	SL	1
Transmission Scan Time	(0013,xx18)	FD	1
Transmission Mask Width	(0013,xx19)	FD	1
Copper Attenuator Thickness	(0013,xx1A)	FD	1
Tomo View Offset	(0013,xx1E)	FD	1-n
Study Comments	(0013,xx26)	LT	1

**This Page Intentionally Left Blank**

## **4. PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL DEFINITION**

### **4.1 INTRODUCTION**

This section specifies the use of the DICOM Patient Root Query/Retrieve Model used to organize data and against which a Query/Retrieve will be performed. The contents of this section are:

4.2 - Information Model Description

4.3- Information Model Entity-Relationship Model

4.4 - Information Model Keys

### **4.2 PATIENT ROOT INFORMATION MODEL DESCRIPTION**

The Patient Root Query/Retrieve Information Model is based upon a four level hierarchy:

Patient  
Study  
Series  
Image

The patient level is the top level and contains Attributes associated with the Patient Information Entity (IE) of Image IODs. Patient IEs are modality independent.

The study level is below the patient level and contains Attributes associated with the Study IE of Image IODs. A study belongs to a single patient. A single patient may have multiple studies. Study IEs are modality independent.

The series level is below the study level and contains Attributes associated with the Series, Frame of Reference and Equipment IEs of Image IODs. A series belongs to a single study. A single study may have multiple series. Series IEs are modality dependent

The lowest level is the image level and contains Attributes associated with the Image IE of Image IODs. An image belongs to a single series. A single series may contain multiple images. Image IEs are modality dependent

### **4.3 PATIENT ROOT INFORMATION MODEL ENTITY-RELATIONSHIP MODEL**

The Entity-Relationship diagram for the Patient Root Information Model schema is shown in Figure 4-1. In this figure, the following diagrammatic convention is established to represent the information organization :

each entity is represented by a rectangular box


each relationship is represented by a diamond shaped box.

the fact that a relationship exists between two entities is depicted by lines connecting the corresponding entity boxes to the relationship boxes.

The relationships are fully defined with the maximum number of possible entities in the relationship shown. In other words, the relationship between Series and Image can

have up to n Images per Series, but the Patient to Study relationship has 1 Study for each Patient (a Patient can have more than one Study on the system, however each Study will contain all of the information pertaining to that Patient).

FIGURE 4-1  
PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL E/R DIAGRAM

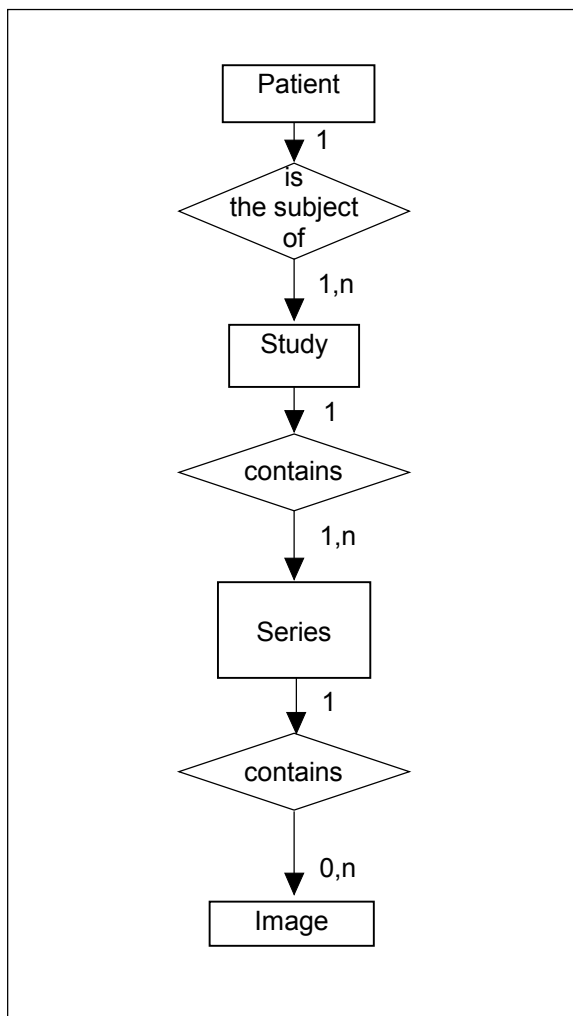

### 4.3.1 ENTITY DESCRIPTIONS

Please refer to the DICOM v3.0 Standard PS 3.4 (Service Class Specifications) for a description of each of the levels contained within the Patient Root Query/Retrieve Information Model.

#### 4.3.1.1 Patient Entity Description

The Patient Entity defines the characteristics of a patient who is the subject of one or more medical studies which produce medical images.

#### 4.3.1.2 Study Entity Description

The Study Entity defines the characteristics of a medical study performed on a patient. A study is a collection of one or more series of medical images which are

logically related for the purpose of diagnosing a patient. Each study is associated with exactly one patient.

**4.3.1.3 Series Entity Description**

The Series Entity defines the attributes which are used to group images into distinct logical sets. Each series is associated with exactly one study.

**4.3.1.4 Image Entity Description**

The Image Entity defines the attributes which describe the pixel data of an image. The pixel data is generated as a direct result of patient scanning (an Original image). An image is defined by its image plane, pixel data characteristics gray scale and/or color mapping characteristics and modality specific characteristics (acquisition parameters and image creation information).

**4.3.2 GENIE Acquisition Mapping of DICOM Entities**

**TABLE 4.3-1**  
**MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES**

DICOM	GENIE Acquisition Entity
Patient	Patient
Study	Study
Series	Series
Image	Imageset

**4.4 INFORMATION MODEL KEYS**

Please refer to the DICOM v3.0 Standard PS 3.4 (Service Class Specifications) for a description of each of the levels contained within the Patient Root Query/Retrieve Information Model.

The following Level descriptions are included to specify which data elements are supported and what type of filtering can be applied. It should be noted that they are the same ones as defined in the DICOM v3.0 Standard PS 3.4 (Service Class Specifications).

**4.4.1 Supported Filtering**

Following are the types of matching that are supported by this implementation :

- Single Value matching
- Wild Card Matching
- Range of date, Range of Time

**4.4.2 Patient Level**

This section defines the keys at the Patient Level of the Patient Root Query/Retrieve Information Model that are supported by this implementation.



DIR 2412345-100 REV 1

TABLE 4.4-1

PATIENT LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	Note
Patient's Name	(0010,0010)	R	Matched. Matching performed without regard to the PN VR individual component values.
Patient ID	(0010,0020)	U	Matched.
Patient Birth Date	(0010,0030)	O	Matched

TABLE 4.4-2

Q/R PATIENT LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES

Attribute Name	Tag	Type	Note
Query Retrieve Level	(0008,0052)	-	Value = PATIENT
Retrieve AE Title	(0008, 0054)	-	Value = AE Title of SCP.

### 4.4.3 Study Level

This section defines the keys at the Study Level of the Patient Root Query/Retrieve Information Model that are supported by this implementation.

TABLE 4.4-3

STUDY LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	Note
Study Date	(0008,0020)	R	Matched.
Study Time	(0008,0030)	R	Matched.
Accession Number	(0008,0050)	R	NOT Matched in GENIE Acquisition R2.3.1 and R2.3.2. Matched in GENIE Acquisition R2.3.3.
Study ID	(0020,0010)	R	Matched.
Study Instance UID	(0020,000D)	U	Matched.
Study Description	(0008,1030)	O	Matched.

TABLE 4.4-4

Q/R STUDY LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES

Attribute Name	Tag	Type	Note
Query Retrieve Level	(0008,0052)	-	Value = STUDY
Retrieve AE Title	(0008, 0054)	-	Value = AE Title of SCP.

### 4.4.4 Series Level

This section defines the keys at the Series Level of the Patient Root Query/Retrieve Information Model that are supported by this implementation.

TABLE 4.4-5

SERIES LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	Note
Modality	(0008,0060)	R	Matched.

Series Number	(0020,0011)	R	Matched.
Series Instance UID	(0020,000E)	U	Matched.
Series Date	(0008,0021)	O	Matched.
Series Time	(0008,0031)	O	Matched.
Series Description	(0008,103E)	O	Returned.

**TABLE 4.4-6  
Q/R SERIES LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES**

Attribute Name	Tag	Type	Note
Query Retrieve Level	(0008,0052)	-	Value = SERIES
Retrieve AE Title	(0008, 0054)	-	Value = AE Title of SCP.

**4.4.5 Image Level**

This section defines the keys at the Image Level of the Patient Root Query/Retrieve Information Model that are supported by this implementation.

**TABLE 4.4-7  
IMAGE LEVEL ATTRIBUTES FOR THE PATIENT ROOT QUERY/RETRIEVE INFORMATION MODEL**

Attribute Name	Tag	Type	Note
Image Number	(0020,0013)	R	Matched.
SOP Instance UID	(0008,0018)	U	Matched.
Image Type	(0008,0008)	O	Returned.
Image ID	(0054,0400)	O	Returned.
Rows	(0028,0010)	O	Returned.
Columns	(0028,0011)	O	Returned.
Number of Frames	(0028,0008)	O	Returned.

**TABLE 4.4-8  
Q/R IMAGE LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES**

Attribute Name	Tag	Type	Note
Query Retrieve Level	(0008,0052)	-	Value = IMAGE
Retrieve AE Title	(0008, 0054)	-	Value = AE Title of SCP.

**4.5 PRIVATE DATA DICTIONARY**

There are no private query key attributes defined for this implementation.

**This Page Intentionally Left Blank**

## **5. STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL DEFINITION**

### **5.1 INTRODUCTION**

This section specifies the use of the DICOM Study Root Query/Retrieve Model used to organize data and against which a Query/Retrieve will be performed. The contents of this section are:

5.2 - Information Model Description

5.3 - Information Model Entity-Relationship Model

5.4 - Information Model Keys

### **5.2 STUDY ROOT INFORMATION MODEL DESCRIPTION**

The Study Root Query/Retrieve Information Model is based upon a three level hierarchy:

Study

Series

Image

The study level is the top level and contains Attributes associated with the Study IE of Image IODs. Attributes of patients are considered to be attributes of studies. Study IEs are modality independent.

The series level is below the study level and contains Attributes associated with the Series, Frame of Reference and Equipment IEs of Image IODs. A series belongs to a single study. A single study may have multiple series. Series IEs are modality dependent

The lowest level is the image level and contains Attributes associated with the Image IE of Image IODs. An image belongs to a single series. A single series may contain multiple images. Image IEs are modality dependent

### **5.3 STUDY ROOT INFORMATION MODEL ENTITY-RELATIONSHIP MODEL**


The Entity-Relationship diagram for the Study Root Information Model schema is shown in Figure 5-1. In this figure, the following diagrammatic convention is established to represent the information organization:

each entity is represented by a rectangular box

each relationship is represented by a diamond shaped box.

the fact that a relationship exists between two entities is depicted by lines connecting the corresponding entity boxes to the relationship boxes.

The relationships are fully defined with the maximum number of possible entities in the relationship shown. In other words, the relationship between Series and Image can have up to n Images per Series.

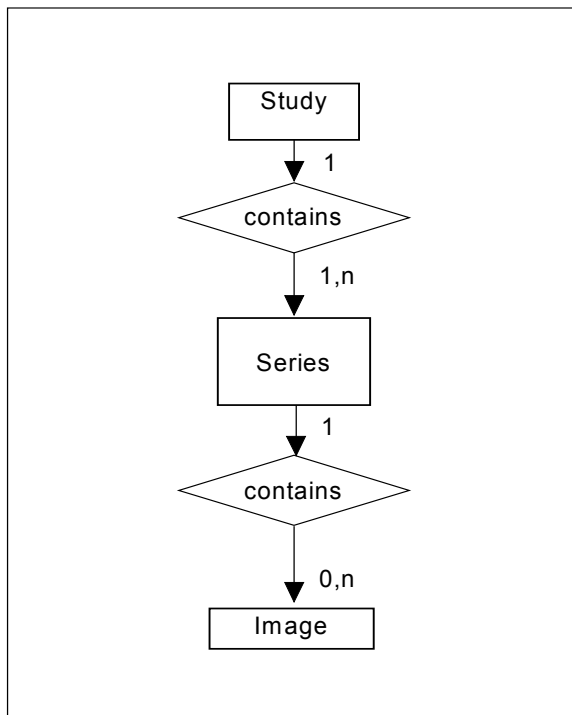

**5.3.1 Entity Descriptions**

Please refer to the DICOM v3.0 Standard PS 3.4 (Service Class Specifications) for a description of each of the levels contained within the Study Root Query/Retrieve Information Model.

**5.3.1.1 Study Entity Description**

The Study Entity defines the characteristics of a medical study performed on a patient. A study is a collection of one or more series of medical images which are logically related for the purpose of diagnosing a patient. Each study is associated with exactly one patient.

**5.3.1.2 Series Entity Description**

The Series Entity defines the attributes which are used to group images into distinct logical sets. Each series is associated with exactly one study.

**5.3.1.3 Image Entity Description**

The Image Entity defines the attributes which describe the pixel data of an image. The pixel data is generated as a direct result of patient scanning (an Original image). An image is defined by its image plane, pixel data characteristics gray scale and/or color mapping characteristics and modality specific characteristics (acquisition parameters and image creation information).

5.3.2 GENIE ACQUISITION Mapping of DICOM Entities

TABLE 5.3-1  
MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES

DICOM	GENIE Acquisition Entity
Study	Study
Series	Series
Image	Imageset

5.4 INFORMATION MODEL KEYS

Please refer to the DICOM v3.0 Standard PS 3.4 (Service Class Specifications) for a description of each of the levels contained within the Study Root Query/Retrieve Information Model.

The following Level descriptions are included to specify what data elements are supported and what type of filtering can be applied. It should be noted that they are the same ones as defined in the DICOM v3.0 Standard PS 3.4 (Service Class Specifications).

5.4.1 Supported Filtering

Following are the types of matching that are supported by this implementation :

- Single Value matching
- Wild Card Matching
- Range of date, Range of Time

5.4.2 Study Level

This section defines the keys at the Study Level of the Study Root Query/Retrieve Information Model that are supported by this implementation.

TABLE 5.4-1  
STUDY LEVEL ATTRIBUTES FOR THE STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	Attribute Description
Study Date	(0008,0020)	R	Matched.
Study Time	(0008,0030)	R	Matched.
Accession Number	(0008,0050)	R	NOT matched in GENIE Acquisition R2.3.1 and R2.3.2. Matched in GENIE Acquisition R2.3.3.
Patient's Name	(0010,0010)	R	Matched. Matching performed without regard to the PN VR individual component values.
Patient ID	(0010,0020)	R	Matched.
Study ID	(0020,0010)	R	Matched.
Study Instance UID	(0020,000D)	U	Matched.
Study Description	(0008,1030)	O	Matched.

**GE MEDICAL SYSTEMS**

**DICOM CONFORMANCE STATEMENT**

DIR 2412345-100 REV 1

**TABLE 5.4-2**

**Q/R STUDY LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES**

Attribute Name	Tag	Type	Note
Query Retrieve Level	(0008,0052)	-	Value = STUDY
Retrieve AE Title	(0008, 0054)	-	Value = AE Title of SCP.

**5.4.3 Series Level**

This section defines the keys at the Series Level of the Study Root Query/Retrieve Information Model that are supported by this implementation.

**TABLE 5.4-3**

**SERIES LEVEL ATTRIBUTES FOR THE STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL**

Attribute Name	Tag	Type	Attribute Description
Modality	(0008,0060)	R	Matched.
Series Number	(0020,0011)	R	Matched.
Series Instance UID	(0020,000E)	U	Matched.
Series Date	(0008,0021)	O	Matched.
Series Time	(0008,0031)	O	Matched.
Series Description	(0008,103E)	O	Returned.

**TABLE 5.4-4**

**Q/R SERIES LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES**

Attribute Name	Tag	Type	Note
Query Retrieve Level	(0008,0052)	-	Value = SERIES
Retrieve AE Title	(0008, 0054)	-	Value = AE Title of SCP.

**5.4.4 Image Level**

This section defines the keys at the Image Level of the Study Root Query/Retrieve Information Model that are supported by this implementation.

**TABLE 5.4-5**

**IMAGE LEVEL ATTRIBUTES FOR THE STUDY ROOT QUERY/RETRIEVE INFORMATION MODEL**

Attribute Name	Tag	Type	Attribute Description
Image Number	(0020,0013)	R	Matched.
SOP Instance UID	(0008,0018)	U	Matched.
Image Type	(0008,0008)	O	Returned.
Rows	(0028,0010)	O	Returned.
Columns	(0028,0011)	O	Returned.
Number of Frames	(0028,0008)	O	Returned.

**TABLE 5.4-6**

**Q/R IMAGE LEVEL AND LOCATION FOR RETRIEVE ATTRIBUTES**

Attribute Name	Tag	Type	Note
Query Retrieve Level	(0008,0052)	-	Value = IMAGE
Retrieve AE Title	(0008, 0054)	-	Value = AE Title of SCP.

There are no private query key attributes defined for this implementation.

**This Page Intentionally Left Blank**



## **6. MODALITY WORKLIST INFORMATION MODEL DEFINITION**

### **6.1 INTRODUCTION**

This section specifies the use of the DICOM Modality Worklist Information Model used to organize data and against which a Modality Worklist Query will be performed. The contents of this section are:

6.2 - Information Model Description

6.3- Information Model Entity-Relationship Model

6.4- Information Model Module Table

6.5- Information Model Keys

### **6.2 MODALITY WORKLIST INFORMATION MODEL DESCRIPTION**

In order to serve as a Service Class User (SCU) of the Modality Worklist service class, a DICOM Application Entity (AE) retrieves information about the attributes of a number of managed worklist items. These items are organised into Modality Worklist Information modules. In this service class, the Information Model plays a role similar to an Information Object Definition of most other DICOM Service Classes.


### **6.3 MODALITY WORKLIST INFORMATION MODEL ENTITY-RELATIONSHIP MODEL**

The Entity-Relationship diagram for the Modality Worklist Information Model schema is shown in Illustration 6.3-1. It represents the information that composes a Worklist Item. In this figure, the following diagrammatic convention is established to represent the information organization :

each entity is represented by a rectangular box

each relationship is represented by a diamond shaped box.

the fact that a relationship exists between two entities is depicted by lines connecting the corresponding entity boxes to the relationship boxes.

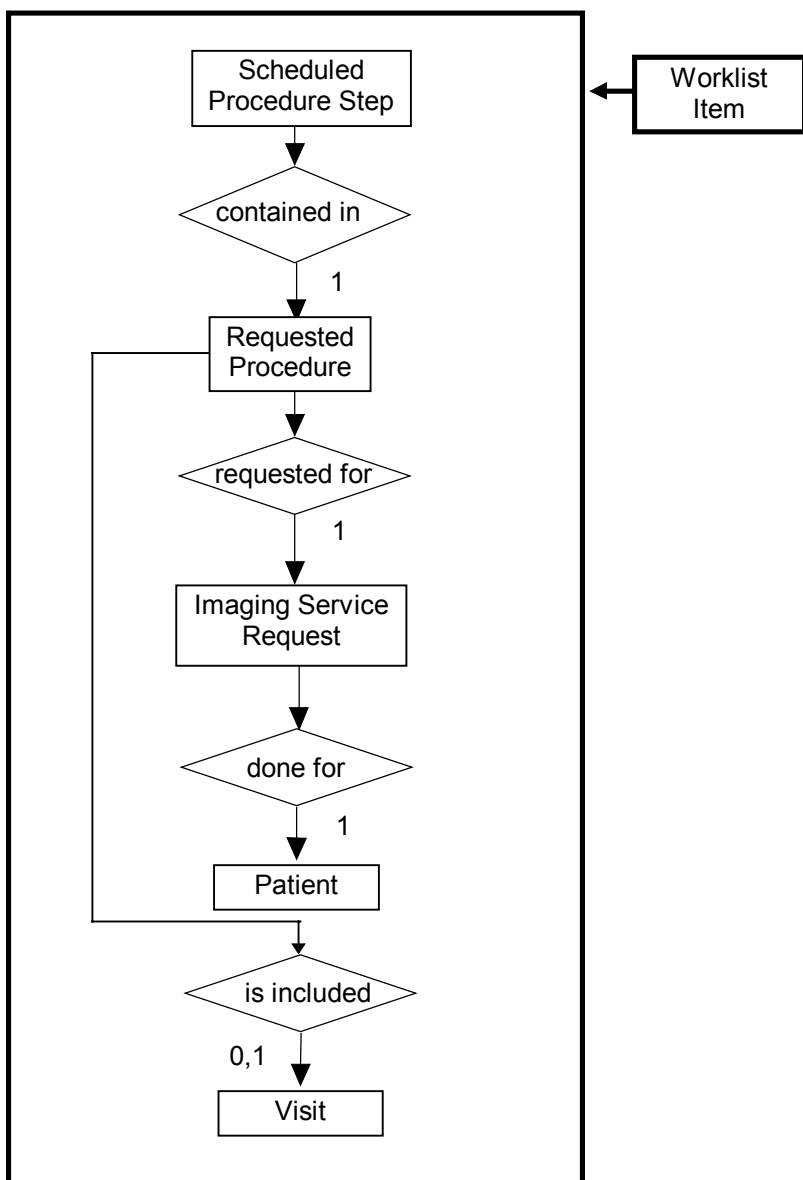

6.3.1 ENTITY DESCRIPTIONS

Please refer to DICOM Standard PS 3.3. (Information Object Definitions) and PS 3.4 (Service Class Specifications) for a description of each of the Entities contained within the Modality Worklist Information Model.

6.3.1.1 Scheduled Procedure Step

A Scheduled Procedure Step is an arbitrarily defined scheduled unit of service that is specified by the Procedure Plan for a Requested Procedure. It specifies one or more Action Items (events) involving equipment (i.e. imaging modality equipment), human resources, location and time (i.e. start time, stop time, duration).

**6.3.1.2 Requested Procedure Entity Description**

A Requested Procedure is an instance of a Procedure of a given Procedure Type. An instance of a Requested Procedure includes all of the items of information that are specified by an instance of a Procedure Plan that is selected for the Requested Procedure by the imaging service provider.

**6.3.1.3 Imaging Service Request Entity Description**

An Imaging Service Request is a set of one or more Requested Procedures selected from a list of Procedure Types. An Imaging Service Request is submitted by one authorized imaging service requester to one authorized imaging service provider in the context of one Service Episode.

**6.3.1.4 Visit Entity Description**

A Visit is the context in which the treatment or management of an arbitrary subset of a Patient's medical conditions occurs. A Visit is limited to the description of a Patient's activities at a single facility.

**6.3.1.5 Patient Entity Description**

A Patient is a person receiving, or registered to receive, healthcare services.

**6.3.2 GENIE Acquisition Mapping of DICOM entities**

**TABLE 6.3-1**  
**MAPPING OF DICOM ENTITIES TO GENIE ACQUISITION ENTITIES**

DICOM	GENIE Acquisition Entity
Scheduled Procedure Step	Prescription (Series)
Requested Procedure	Prescription (Series) / Study
Imaging Service Request	Study
Visit	Study
Patient	Patient

**6.4 INFORMATION MODEL MODULE TABLE**

Within an entity of the DICOM v3.0 Modality Worklist Information Model, attributes are grouped into related set of attributes. A set of related attributes is termed a module. A module facilitates the understanding of the semantics concerning the attributes and how the attributes are related with each other. A module grouping does not infer any encoding of information into datasets.

Table 1.4-1 identifies the defined modules within the entities which comprise the DICOM v3.0 Modality Worklist Information Model. Modules are identified by Module Name.

See DICOM v3.0 PS 3.3 and PS 3.4 for a complete definition of the entities, modules, and attributes.

**TABLE 6.4-1**  
**MODALITY WORKLIST INFORMATION MODEL MODULES**

Entity Name	Module Name	Reference
Scheduled Procedure Step	SOP Common	6.5.2.1
	Scheduled Procedure Step	6.5.2.2
Requested Procedure	Requested Procedure	6.5.3.1
Imaging Service Request	Imaging Service Request	6.5.4.1
Visit	Visit Identification	6.5.5.1
	Visit Status	6.5.5.2
	Visit Relationship	6.5.5.3
	Visit Admission	6.5.5.4
Patient	Patient Relationship	6.5.6.1
	Patient Identification	6.5.6.2
	Patient Demographic	6.5.6.3
	Patient Medical	6.5.6.4

**6.5 INFORMATION MODEL KEYS**

Please refer to DICOM Standard PS 3.3. (Information Object Definitions) and PS 3.4 (Service Class Specifications) for a description of each of the Entities contained within the Modality Worklist Information Model.

The following Module descriptions are included to specify what data elements are supported and what type of matching can be applied. It should be noted that they are the same ones as defined in the DICOM v3.0 Standard PS 3.4 (Service Class Specifications). A row of each table describes:

Attribute Name

Tag (Group, Element)

Expected Matching Key Type (R-required, O-optional)

Expected Returned Key Type:

1 non-zero value required

1C conditionally of type 1

2 required to be present, possibly zero-length

2C conditionally of type 2

3 optional

Mapped Into The Image (field mapped into Image transfers)

Notes (clarification of this implementation's use/treatment of this attribute)

All of the attributes listed are included in the Modality Worklist query.

**6.5.1 Supported Matching**

Following are the types of matching that can be requested by the implementation :

Single Value matching

Universal Matching

Wild Card Matching

Range of date, Range of Time

6.5.2 Scheduled Procedure Step Entity

6.5.2.1 SOP Common Module

TABLE 6.5-6.5-1  
SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Specific Character Set	(0008,0005)	O	1C	No	Matching is supported, the matching value=ISO_IR100 is fixed.

6.5.2.2 Scheduled Procedure Step Module

TABLE 6.5-6.5-2  
SCHEDULED PROCEDURE STEP MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Scheduled Procedure Step Sequence	(0040,0100)	R	1	No	
>Scheduled Station AE Title	(0040,0001)	R	1	No	Matching supported. Universal or Single Value. If user specifies a station name then it's AE title is determined from configuration.
>Scheduled Procedure Step Start Date	(0040,0002)	R	1	No	Matching Supported. Specified as range of date of the form: Date-Date where Date can be specified as one of: yyymmdd or *
>Scheduled Procedure Step Start Time	(0040,0003)	R	1	No	Matching supported. Specified as time range of time of the form: Time1-Time2 where time can be specified as: hhmmss.frac or *
>Scheduled Procedure Step End Date	(0040,0004)	O	3	No	
>Scheduled Procedure Step End Time	(0040,0005)	O	3	No	

DIR 2412345-100 REV 1

>Modality	(0008,0060)	R	1	No	Matching Supported. Single value matching performed. Images transferred always have Value=NM
>Scheduled Performing Physician's Name	(0040,0006)	R	2	Yes	Matching Supported. Universal, Single or Wildcard. Mapped to image field (0008, 1050) performing physicians name.
>Scheduled Procedure Step Description	(0040,0007)	O	1C	No	
>Scheduled Station Name	(0040,0010)	O	2	No	Matching supported. Universal or Single Value. Used in conjunction with (0040,0001) Scheduled Station AE Title.
>Pre-Medication	(0040,0012)	O	2C	No	
>Scheduled Procedure Step ID	(0040,0009)	O	1	No	Matching Supported. Universal, Single or Wildcard.
>Requested Contrast Agent	(0032,1070)	O	2C	No	
>Scheduled Procedure Step Status	(0040,0020)	O	3	No	
>Comments on the Scheduled Procedure Step	(0040,0400)	O	3	No	

6.5.3 Requested Procedure Entity

6.5.3.1 Requested Procedure Module

TABLE 6.5-6.5-3  
REQUESTED PROCEDURE MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Requested Procedure ID	(0040,1001)	O	1	No	Matching supported. Universal, Single value, Wildcard.
Requested Procedure Description	(0032,1060)	O	1C	No	
Study Instance UID	(0020,000D)	O	1	Yes	
Requested Procedure Priority	(0040,1003)	O	2	No	
Patient Transport Arrangements	(0040,1004)	O	2	No	
Reason for the Requested Procedure	(0040,1002)	O	3	No	
Requested Procedure Comments	(0040,1400)	O	3	No	
Requested Procedure Location	(0040,1005)	O	3	No	

DIR 2412345-100 REV 1

Names of Intended Recipients Of Results	(0040,1010)	O	3	Yes	Mapped to image field (0008,1060) Names of Physicians Reading Study
---	-------------	---	---	-----	---

6.5.4 Imaging Service Request Entity

6.5.4.1 Imaging Service Request Module

TABLE 6.5-6.5-4  
IMAGING SERVICE REQUEST MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Accession Number	(0008,0050)	O	2	Yes	Matching Supported. Universal, Single Value, Wildcard.
Requesting Physician	(0032,1032)	O	2	No	
Referring Physician's Name	(0008,0090)	O	2	Yes	
Reason for the Imaging Service Request	(0040,2001)	O	3	No	
Imaging Service Request Comments	(0040,2400)	O	3	No	

6.5.5 Visit Entity

6.5.5.1 Visit Identification

TABLE 6.5-6.5-5  
VISIT IDENTIFICATION MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
None Defined					



6.5.5.2 Visit Status

TABLE 6.5-6.5-6  
VISIT STATUS MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Current Patient Location	(0038,0300)	O	2	No	

6.5.5.3 Visit Relationship

TABLE 6.5-6.5-7  
VISIT RELATIONSHIP MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
None Defined					

6.5.5.4 Visit Admission

TABLE 6.5-6.5-8  
VISIT ADMISSION MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Admitting Diagnosis Description		O	3	Yes	

6.5.6 Patient Entity

6.5.6.1 Patient Relationship

TABLE 6.5-6.5-9  
PATIENT RELATIONSHIP MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
None Defined					

**6.5.6.2 Patient Identification**

**TABLE 6.5-6.5-10**  
**PATIENT IDENTIFICATION MODULE ATTRIBUTES**

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Patient's Name	(0010,0010)	R	1	Yes	Matching Supported. Universal, Single Value or Wildcard. User can query using full definition of VR_PN.
Patient ID	(0010,0020)	R	1	Yes	Matching Supported. Single Value matching.
Other Patient Ids	(0010,1000)	O	3	Yes	
Other Patient Names	(0010,1001)	O	3	Yes	

**6.5.6.3 Patient Demographic**

**TABLE 6.5-6.5-11**  
**PATIENT DEMOGRAPHIC MODULE ATTRIBUTES**

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into the Image	Note
Patients Birth Date	(0010,0030)	O	2	Yes	
Patient's Sex	(0010,0040)	O	2	Yes	
Patient's Weight	(0010,1030)	O	2	Yes	
Patient's Size	(0010,1020)	O	3	Yes	
Patient's Age	(0010,1010)	O	3	Yes	
Occupation	(0010,2180)	O	3	Yes	
Ethnic Group	(0010,2160)	O	3	Yes	
Patient Comments	(0010,4000)	O	3	Yes	

**6.5.6.4 Patient Medical**

**TABLE 6.5-6.5-12**  
**PATIENT MEDICAL MODULE ATTRIBUTES**

<b>Attribute Name</b>	<b>Tag</b>	<b>Expected Matching Key Type</b>	<b>Expected Returned Key Type</b>	<b>Mapped into the Image</b>	<b>Note</b>
Patient State	(0038,0500)	O	2	No	
Pregnancy Status	(0010,21C0)	O	2	No	
Medical Alerts	(0010,2000)	O	2	No	
Contrast Allergies	(0010,2110)	O	2	No	
Special Needs	(0038,0050)	O	2	No	
Additional Patient History	(0010,21B0)	O	3	Yes	

**6.6 PRIVATE DATA DICTIONARY**

The Type of a Private Attribute is determined by the level of the Information Model in which it is used, and hence is not listed in this dictionary. Any Private Attribute contained within the Information Model is described in the preceding sections in the appropriate level.

NO PRIVATE ATTRIBUTES ARE DEFINED.

## **7. XELERIS/ENTEGR A PROTOCOL DATA INFORMATION OBJECT DEFINITION**

### **7.1 INTRODUCTION**

Ignite is a feature that enables an operator to request a remote AE (namely Xeleris) to process acquired data. The acquisition station holds an imported list of the processing protocols offered by one or more processing stations. When defining an acquisition protocol or setting up a study, the acquisition station user selects the processing protocols to be applied to that study. After all the required data is acquired and transferred, the acquisition station sends a processing request to the processing station.

This section specifies the use of the Private DICOM Xeleris/eNTEGRA Information Object. The contents of this section are:

7.2 - Xeleris/eNTEGRA PROTOCOL DATA IOD IMPLEMENTATION

7.3 - IOD MODULE TABLE

7.4 - information module definitions

### **7.2 XELERIS/ENTEGR A PROTOCOL DATA IOD IMPLEMENTATION**

The Xeleris/eNTEGRA Protocol Data Information Objects are used for storage of image processing data that are beyond image attributes. A protocol data object is associated with a Study, and not associated with a series or an Image. For this reason a stand-alone private object is defined for transferring protocol data between GEMS acquisition and processing systems.

### **7.3 IOD MODULE TABLE**

This section defines a Xeleris/eNTEGRA Private Protocol Data Object that consists of the DICOM standard Patient, Study, Series and SOP common modules and the Xeleris/eNTEGRA Private Protocol Data Module. The private module is based on the Protocol Data Table that is defined in Xeleris/eNTEGRA database schema document.

The Xeleris/eNTEGRA Private Protocol Data Object Module Table is shown below.

The GENIE Acquisition private data dictionary will be extended to show the value representation and other characteristics shown in the table.

TABLE 7.3-1

XELERIS/eNTEGRA PROTOCOL DATA IOD MODULES

Entity Name	Module Name	Reference
Patient	Patient	7.4.16.5.2.1
	GENIE Acquisition Patient	
Study	General Study	7.4.1.2
	Patient Study	
	GENIE Acquisition Study	
Series	General Series	7.4.3
Xeleris/eNTEGRA Data	Xeleris/eNTEGRA Protocol Data	7.4.4
	SOP Common	7.4.5

7.4 INFORMATION MODULE DEFINITIONS

The following table shows the Private Xeleris/eNTEGRA Protocol Data Information Object fields that are sent by GENIE Acquisition.

7.4.1 Patient Entity Modules

7.4.1.1 Patient Module

This section specifies the Attributes which identify and describe general information about the Patient.

TABLE 7.4-1

PATIENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Patient's Name	(0010,0010)	2	Set to "PHYSICIAN INBOX"
Patient ID	(0010,0020)	2	Set to "PHYSICIAN INBOX"
Patient's Birth Date	(0010,0030)	2	Not Used.
Patient's Sex	(0010,0040)	2	Set to "M"
Referenced Patient Sequence	(0008,1120)	3	Not Used.
>Referenced SOP Class UID	(0008,1150)	1C	Not Used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not Used.
Patient's Birth Time	(0010,0032)	3	Not Used.
Other Patient Ids	(0010,1000)	3	Not Used.
Other Patient Names	(0010,1001)	3	Not Used.
Ethnic Group	(0010,2160)	3	Not Used.
Patient Comments	(0010,4000)	3	Not Used.

7.4.1.2 GENIE Acquisition Patient Module Attributes

This section specifies the Attributes which identify and describe the patient who is the subject of a diagnostic study. This module contains *private* Attributes that convey information not contained in similar DICOM standard v3.0 module(s).

TABLE 7.4-2  
GENIE ACQUISITION PATIENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Patient Object Name	(0009,xx40)	3	Set to "PHYSICIAN INBOX"
Patient Flags	(0009,xx41)	3	Set to 1 (Complete)
Patient Creation Date	(0009,xx42)	3	Not Used.
Patient Creation Time	(0009,xx43)	3	Not Used.

7.4.2 Study Entity Modules

7.4.2.1 General Study Module

This section specifies the Attributes which identify and describe general information about the Study within a Patient.

TABLE 7.4-3  
GENERAL STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Study Instance UID	(0020,000D)	1	Set to "1.2.840.113619.2.175.0.0.1.1"
Study Date	(0008,0020)	2	Creation date of study entity (yyyymmdd)
Study Time	(0008,0030)	2	Creation time of study entity (hhmmss)
Referring Physician's Name	(0008,0090)	2	Not Used.
Study ID	(0020,0010)	2	Set to "MILLENNIUM"
Accession Number	(0008,0050)	2	Not Used.
Study Description	(0008,1030)	3	Entered on To Do card, Study Name field
Physician(s) of Record	(0008,1048)	3	Not Used.
Name of Physician(s) Reading Study	(0008,1060)	3	Not Used.
Referenced Study Sequence	(0008,1110)	3	Not Used.
>Referenced SOP Class UID	(0008,1150)	1C	Not Used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not Used.
Procedure Code Sequence	(0008,1032)	3	Not Used.
>Code Value	(0008,0100)	1C	Not Used.
>Coding Scheme Designator	(0008,0102)	1C	Not Used.
>Coding Scheme Version	(0008,0104)	1C	Not Used.

7.4.2.2 Patient Study Module

This section specifies the Attributes about the patient at the time the study was performed.

TABLE 7.4-4  
PATIENT STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Admitting Diagnoses Description	(0008,1080)	3	Not Used.
Patient's Age	(0010,1010)	3	Not Used.
Patient's Size	(0010,1020)	3	Not Used.
Patient's Weight	(0010,1030)	3	Not Used.
Occupation	(0010,2180)	3	Not Used.
Additional Patient's History	(0010,21BO)	3	Not Used.

7.4.2.3 GENIE Acquisition Study Module

This section specifies the Attributes which describe and identify the study performed upon the Patient. The module contains *private* Attributes that convey information not contained in similar DICOM standard v3.0 Modules(s).

TABLE 7.4-5  
GENIE ACQUISITION STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Study Name	(0009,xx10)	3	Set to "MILLENNIUM"
Study Flags	(0009,xx11)	3	Set to 513 (Complete & Hidden)
Study Type	(0009,xx12)	3	Set to 0
Study Comments	(0013,xx26)	3	Not Used.

7.4.3 General Series Module

This section specifies the Attributes which identify and describe general information about the Series within a Study.

This is Not Used.

7.4.4 Xeleris/eNTEGRA Protocol Data

This section specifies the Attributes which identify and describe information about the protocol data.

TABLE 7.4-6  
XELERIS/ENTEGR A PROTCOL DATA ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Xeleris/eNTEGRA Data Object Type	(0033,xx08)	-	Set to "PROTOCOL DATA"
Modified	(0033,xx10)	-	Not Used.
Name	(0033,xx11)	-	Set to "MILLENNIUM"
Protocol Data UID	(0033,xx16)	-	Internally generated.
Date	(0033,xx17)	-	Processing Request date (yyyymmdd)
Time	(0033,xx18)	-	Processing Request time (hhmmss)
Protocol Data Flags	(0033,xx19)	-	Set to 8193 (0x2001 Waiting & Auto-Start)
Protocol Name	(0033,xx1A)	-	Set to "PHYSICIAN INBOX TASK"
Relevant Data UID	(0033,xx1B)	-	Set to "Test"
Bulk Data	(0033,xx1C)	-	Task Information String
Int Data	(0033,xx1D)	-	Not Used
Double Data	(0033,xx1E)	-	Not Used
String Data	(0033,xx1F)	-	Set to "1.2.840.113619.2.175.0.0.1,1"
Bulk Data Format	(0033,xx20)	-	Set to "task_info\688"
Int Data Format	(0033,xx21)	-	Not Used.
Double Data Format	(0033,xx22)	-	Not Used.
String Data Format	(0033,xx23)	-	Set to "data_uid_list\1"
Description	(0033,xx24)	-	Not Used.
SDO Double Data SQ	(0033,xx64)	-	Not Used.
Double Data	(0033,xx1E)	-	Not Used.

7.4.5 SOP Common Module

This section defines the Attributes which are required for proper functioning and identification of the associated SOP Instances. They do not specify any semantics about the Real-World Object represented by the IOD.

TABLE 7.4-7  
SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
SOP Class UID	(0008,0016)	1	Set to "1.2.840.113619.4.27"
SOP Instance UID	(0008,0018)	1	Internally generated.
Specific Character Set	(0008,0005)	1C	Set to "ISO_IR 100"
Instance Creation Date	(0008,0012)	3	Not Used.
Instance Creation Time	(0008,0013)	3	Not Used.
Instance Creator UID	(0008,0014)	3	Not Used.



7.5 PRIVATE DATA DICTIONARY

This section provides value representation and multiplicity information for all of the Private Attributes used by this implementation. Private Attributes contained within the Information Model are described in the preceding sections.

TABLE 7.5-1  
PRIVATE CREATOR IDENTIFICATION (GEMS\_GENIE\_1)

Attribute Name	Tag	VR	VM
Patient Object Name	(0009,xx40)	PN	
Patient Flags	(0009,xx41)	SL	1
Study Name	(0009,xx10)	LO	1
Study Flags	(0009,xx11)	SL	1
Study Type	(0009,xx12)	SL	1
Study Comments	(0013,xx26)	LT	0
Data Object Type	(0033, xx08)	CS	13
Protocol Data Name	(0033, xx11)	LO	1
Protocol data UID	(0033,xx16)	LO	1
Protocol Data Date	(0033,xx17)	SH	1
Protocol Data Time	(0033,xx18)	SH	1
Protocol Data Flags	(0033,xx19)	UL	1
Protocol Name	(0033,xx1A)	LO	1
Bulk Data	(0033,xx1B)	OB	
Relevant Series	(0033,xx1B)	LO	4
Int Data	(0033,xx1D)	SL	0
Double Data	(0033,xx1E)	FD	0
String Data	(0033,xx1F)	LT	
Bulk Data Format	(0033, xx20)	LT	14
String Data Format	(0033,xx23)	LT	16
Protocol Data Description	(0033,xx24)	LT	0

## **8. STORAGE COMMITMENT PUSH MODEL SOP CLASS DEFINITION**

### **8.1 INTRODUCTION**

This section of the DICOM Conformance Statement specifies the Storage Commitment Push Model SOP Class, the optional attributes and service elements supported, the valid range of values for mandatory and optional attributes, and the status code behaviour.

### **8.2 STORAGE COMMITMENT PUSH MODEL SOP CLASS DEFINITION**

#### **8.2.1 IOD Description**

In order to serve as a Service Class User (SCU) of the Storage Commitment Push Model service class, a DICOM Application Entity (AE) determines the time at which the SOP instances are transmitted. The DICOM AE transmits the SOP instances to the Service Class Provider (SCP) using an appropriate mechanism. The request for Storage Commitment is transmitted to the SCP together with a list of one or more SOP instances. Success or failure of storage commitment is subsequently indicated by a notification by the SCP to the DICOM AE

#### **8.2.1.1 STORAGE COMMITMENT MODULE**

**TABLE 8.2-1 STORAGE COMMITMENT MODULE**

<b>Attribute Name</b>	<b>Tag</b>	<b>Attribute Description</b>
Transaction UID	(0008,1195)	Internally generated
Retrieve AE Title	(0008,0054)	Not used.
Storage Media File-Set ID	(0088,0130)	Not used.
Storage Media File-Set UID	(0088,0140)	Not used.
Referenced SOP Sequence	(0008,1199)	
>Referenced SOP Class UID	(0008,1150)	1.2.840.10008.5.1.4.1.1.20 Nuclear Medicine Image Storage SOP Class UID.
>Referenced SOP Instance UID	(0008,1155)	Internally generated.
>Retrieve AE Title	(0008,0054)	Not used.
>Storage Media File-Set ID	(0088,0130)	Not used.
>Storage Media File-Set UID	(0088,0140)	Not used.
Referenced Study Component Sequence	(0008,1111)	Not used.
>Referenced SOP Class UID	(0008,1150)	Not used.
>Referenced SOP Instance UID	(0008,1155)	Not used.
Failed SOP Sequence	(0008,1198)	

**GE MEDICAL SYSTEMS**

**DICOM CONFORMANCE STATEMENT**

DIR 2412345-100 REV 1

>Referenced SOP Class UID	(0008,1150)	1.2.840.10008.5.1.4.1.1.20 Nuclear Medicine Image Storage SOP Class UID.
>Referenced SOP Instance UID	(0008,1155)	Internally generated.
>Failure Reason	(0008,1197)	Accepts all failure reasons

**TABLE 8.2-2 FAILURE REASON VALUES AND SEMANTICS**

<b>Failure Reason</b>	<b>Meaning</b>	<b>SCU Behavior</b>
0110H	Processing failure	Error logged
0112H	No such object instance	Error logged
0213H	Resource limitation	Error logged
0122H	Referenced SOP Class not supported	Error logged
0119H	Class / Instance conflict	Error logged
0131H	Duplicate transaction UID	Error logged

**8.2.2 DIMSE Service Group**

<b>DIMSE Service Element</b>	<b>Usage SCU/SCP</b>
N-EVENT-REPORT	M/M
N-ACTION	M/M

**8.2.3 Operations**

**8.2.3.1 Action Information**

**TABLE 8.2- STORAGE COMMITMENT REQUEST - ACTION INFORMATION**

<b>Action Type Name</b>	<b>Action Type ID</b>	<b>Attribute</b>	<b>Tag</b>	<b>Requirement Type SCU/SCP</b>
Request Storage Commitment	1	Transaction UID	(0008,1195)	1/1
		Storage Media File-Set ID	(0088,0130)	Not used.
		Storage Media File-Set UID	(0088,0140)	Not used.
		Referenced SOP Sequence	(0008,1199)	1/1
		>Referenced SOP Class UID	(0008,1150)	1/1
		>Referenced SOP Instance UID	(0008,1155)	1/1
		>Storage Media File-Set ID	(0088,0130)	Not used.
		>Storage Media File-Set UID	(0088,0140)	Not used.
		Referenced Study Component Sequence	(0008,1111)	Not used.
		>Referenced SOP Class UID	(0008,1150)	Not used.
>Referenced SOP Instance UID	(0008,1155)	Not used.		

8.2.4.1 Event Information

TABLE 8.2-4 STORAGE COMMITMENT RESULT - EVENT INFORMATION

Event Type Name	Event Type ID	Attribute	Tag	Requirement Type SCU/SCP
Storage Commitment Request Successful	1	Transaction UID	(0008,1195)	-/1
		Retrieve AE Title	(0008,0054)	Not used.
		Storage Media File-Set ID	(0088,0130)	Not used
		Storage Media File-Set UID	(0088,0140)	Not used
		Referenced SOP Sequence	(0008,1199)	-/1
		>Referenced SOP Class UID	(0008,1150)	-/1
		>Referenced SOP Instance UID	(0008,1155)	-/1
		>Retrieve AE Title	(0008,0054)	Not used.
		>Storage Media File-Set ID	(0088,0130)	Not used
		>Storage Media File-Set UID	(0088,0140)	Not used
Storage Commitment Request Complete - Failures Exist	2	Transaction UID	(0008,1195)	-/1
		Retrieve AE Title	(0008,0054)	Not used.
		Storage Media File-Set ID	(0088,0130)	Not used
		Storage Media File-Set UID	(0088,0140)	Not used
		Referenced SOP Sequence	(0008,1199)	-/1C
		>Referenced SOP Class UID	(0008,1150)	-/1
		>Referenced SOP Instance UID	(0008,1155)	-/1
		>Retrieve AE Title	(0008,0054)	Not used.
		>Storage Media File-Set ID	(0088,0130)	Not used
		>Storage Media File-Set UID	(0088,0140)	Not used
		Failed SOP Sequence	(0008,1198)	-/1
		>Referenced SOP Class UID	(0008,1150)	-/1
		>Referenced SOP Instance UID	(0008,1155)	-/1
		>Failure Reason	(0008,1197)	-/1

## 9. SECONDARY CAPTURE INFORMATION OBJECT IMPLEMENTATION

### 9.1 SECONDARY CAPTURE IOD MODULE TABLE

The Secondary Capture Information Object Definition comprises the modules of the following table. Common modules are described in Section 3.5. SC-specific modules are described in Section 7.3. There are no Standard Extended and Private attributes in this implementation.

**TABLE 9.1-1 SC IMAGE IOD MODULES**

Entity Name	Module Name	Usage	Reference
Patient	Patient	Used	9.2.1
Study	General Study	Used	9.2.2
	Patient Study	Used	9.2.3
Series	General Series	Used	9.2.4
Equipment	General Equipment	Used	9.2.5
	SC Equipment	Used	9.2.6
Image	General Image	Used	9.2.7
	Image Pixel	Used	9.2.8
	SC Image	Used	9.2.9
	Overlay Plane	Not Used	
	Modality LUT	Not Used	
	VOI LUT	Not Used	
	SOP Common	Used	9.2.10

### 9.2 INFORMATION MODULE DEFINITIONS

Please refer to DICOM v3.0 Standard Part 3 (Information Object Definitions) for a description of each of the entities and modules contained within the SC Information Object.

9.2.1 Patient Identification Module

TABLE 9.2-1 PATIENT IDENTIFICATION MODULE ATTRIBUTES

Attribute Name	Tag	Type	Note
Patient's Name	(0010,0010)	1	set to "!"Screen Capture"
Patient ID	(0010,0020)	1	Set to the name of station data acquired on.
Other Patient Ids	(0010,1000)	3	Not Used
Other Patient Names	(0010,1001)	3	Not Used

9.2.2 General Study Module

TABLE 9.2-2 GENERAL STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Study Instance UID	(0020,000D)	1	Internally generated
Study Date	(0008,0020)	2	Creation date of study entity (yyyymmdd).
Study Time	(0008,0030)	2	Creation time of study entity (hhmmss).
Referring Physician's Name	(0008,0090)	2	Not used.
Study ID	(0020,0010)	2	Set to "SCRCAP"
Accession Number	(0008,0050)	2	Not used.
Study Description	(0008,1030)	3	Set to "!"SCREEN CAPTURE "
Physician(s) of Record	(0008,1048)	3	Not used.
Name of Physician(s) Reading Study	(0008,1060)	3	Not used.
Referenced Study Sequence	(0008,1110)	3	Not used.
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
Procedure Code Sequence	(0008,1032)	3	Not used.
>Code Value	(0008,0100)	1C	Not used.
>Coding Scheme Designator	(0008,0102)	1C	Not used.
>Coding Scheme Version	(0008,0104).	1C	Not Used

9.2.3 Patient Study Module

TABLE 9.2-3  
PATIENT STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Admitting Diagnoses Description	(0008,1080)	3	Not Used.
Patient's Age	(0010,1010)	3	Not Used.
Patient's Size	(0010,1020)	3	Not Used.
Patient's Weight	(0010,1030)	3	Not Used.
Occupation	(0010,2180)	3	Not Used.
Additional Patient's History	(0010,21BO)	3	Not Used.

9.2.4 General Series Module Attributes

TABLE 9.2-7 GENERAL SERIES MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Modality	(0008,0060)	1	Set to "NM"
Series Date	(0008,0021)	3	Date the Series started.
Series Time	(0008,0031)	3	Time the Series started.
Series Description	(0008,103E)	3	Set To "ScrCap_<num>" where num is a sequential number starting from 1

9.2.5 General Equipment Module

TABLE 9.2-4  
GENERAL EQUIPMENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Manufacturer	(0008,0070)	2	Set to "GE MEDICAL SYSTEMS".
Institution Name	(0008,0080)	3	Set to value displayed on user interface banner.
Institution Address	(0008,0081)	3	Not used.
Station Name	(0008,1010)	3	Set to the name of station data acquired on.
Institutional Department Name	(0008,1040)	3	Not used.
Manufacturer's Model Name	(0008,1090)	3	Set to system type data acquired on.
Device Serial Number	(0018,1000)	3	Set to serial number data acquired on.
Software Versions	(0018,1020)	3	Set to GENIE Acquisition software version.
Spatial Resolution	(0018,1050)	3	Not used.
Date of Last Calibration	(0018,1200)	3	Not used.
Time of Last Calibration	(0018,1201)	3	Not used.
Pixel Padding Value	(0028,0120)	3	Not used.

9.2.6 SC Equipment Module

TABLE 9.2-5 SC IMAGE EQUIPMENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Use
Conversion Type	(0008,0064)	1	Set to "WSD" (Workstation)
Modality	(0008,0060)	3	Set to "NM"
Manufacturer	(0008,0070)	2	Set to "GE MEDICAL SYSTEMS"
Institution Name	(0008,0080)	3	Set to value displayed on user interface banner.
Station Name	(0008,1010)	3	Set to the name of station data acquired on.
Manufacturer's Model Name	(0008,1090)	3	Set to system type data acquired on. e.g. "Millenium MCV"
Device Serial Number	(0018,1000)	3	Set to serial number station data acquired on.
Software Versions	(0018,1020)	3	Software Versions
Secondary Capture Device ID	(0018,1010)	3	Not Used



Secondary Capture Device Manufacturer	(0018,1016)	3	Not Used
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	3	Not Used
Secondary Capture Device Software Version	(0018,1019)	3	Not Used
Video Image Format Acquired	(0018,1022)	3	Not Used
Digital Image Format Acquired	(0018,1023)	3	Not Used

9.2.7 General Image Module

TABLE 9.2-6  
GENERAL IMAGE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Image Number	(0020,0013)	2	Internally generated.
Patient Orientation	(0020,0020)	2C	Not used.
Content Date	(0008,0023)	2C	Date of station data acquisition completion (yyyymmdd).
Content Time	(0008,0033)	2C	Time of station data acquisition completion (hhmmss).
Image Type	(0008,0008)	3	Set to "DERIVEDSECONDARY"
Acquisition Number	(0020,0012)	3	Not used.
Acquisition Date	(0008,0022)	3	Date of station data acquisition completion. (yyyymmdd).
Acquisition Time	(0008,0032)	3	Time of station data acquisition completion. (hhmmss).
Acquisition Datetime	(0008,002A)	3	Not used.
Referenced Image Sequence	(0008,1140)	3	Not Used
>Referenced SOP Class UID	(0008,1150)	1C	Not Used
>Referenced SOP Instance UID	(0008,1155)	1C	Not used
>Referenced Frame Number	(0008,1160)	3	Not used.
Derivation Description	(0008,2111)	3	Not used.
Source Image Sequence	(0008,2112)	3	Not used..
>Referenced SOP Class UID	(0008,1150)	1C	Not used.
>Referenced SOP Instance UID	(0008,1155)	1C	Not used.
>Referenced Frame Number	(0008,1160)	3	Not used.
Images in Acquisition	(0020,1002)	3	Not used
Image Comments	(0020,4000)	3	Not used.
Quality Control Image	(0020,4000)	3	Not used.
Burned In Annotation	(0028,0301)	3	Not used.
Lossy Image Compression	(0028,2110)	3	Set to "00"
Lossy Image Compression Ratio	(0028,2112)	3	Not used.

9.2.8 Image Pixel Module

Table 9.2-7 IMAGE PIXEL MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Samples per Pixel	(0028,0002)	1	Number of samples (planes) in this image. Set to 3 (RGB)
Photometric Interpretation	(0028,0004)	1	Specifies the intended interpretation of the pixel data. Set to "RGB "

Rows	(0028,0010)	1	Number of rows in the image.
Columns	(0028,0011)	1	Number of columns in the image
Bits Allocated	(0028,0100)	1	Number of bits allocated for each pixel sample. Each sample shall has the same number of bits allocated. Set to 8
Bits Stored	(0028,0101)	1	Number of bits stored for each pixel sample. Each sample has the same number of bits stored. Set to 8
High Bit	(0028,0102)	1	Most significant bit for pixel sample data.Each sample has the same high bit. Set to 7
Pixel Representation	(0028,0103)	1	Data representation of the pixel samples. Set to 0 (unsigned integer.)
Pixel Data	(7FE0,0010)	1	A data stream of the pixel samples that comprise the Image.
Planar Configuration	(0028,0006)	1C	Set to 0 (The pixel data are sent color-by-pixel.)
Pixel Aspect Ratio	(0028,0034)	1C	Not Used
Smallest Image Pixel Value	(0028,0106)	3	Not Used
Largest Image Pixel Value	(0028,0107)	3	Not Used

9.2.9 SC Image Module

TABLE 9.2-8 SC IMAGE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Use
Date of Secondary Capture	(0018,1012)	3	Not Used
Time of Secondary Capture	(0018,1014)	3	Not Used

9.2.10 SOP Common Module

TABLE 9.2-9 SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
SOP Class UID	(0008,0016)	1	Set to "1.2.840.10008.5.1.4.1.1.7", Secondary capture Storage SOP Class UID.
SOP Instance UID	(0008,0018)	1	Internally generated
Specific Character Set	(0008,0005)	1C	"ISO_IR 100".
Instance Creation Date	(0008,0012)	3	Not Used
Instance Creation Time	(0008,0013)	3	Not Used
Instance Creator UID	(0008,0014)	3	Not Used

9.3 STANDARD EXTENDED AND PRIVATE DATA ATTRIBUTES

There are no Private key Attrib