





OPTIMA CT660/660Pro w/1700 TABLE

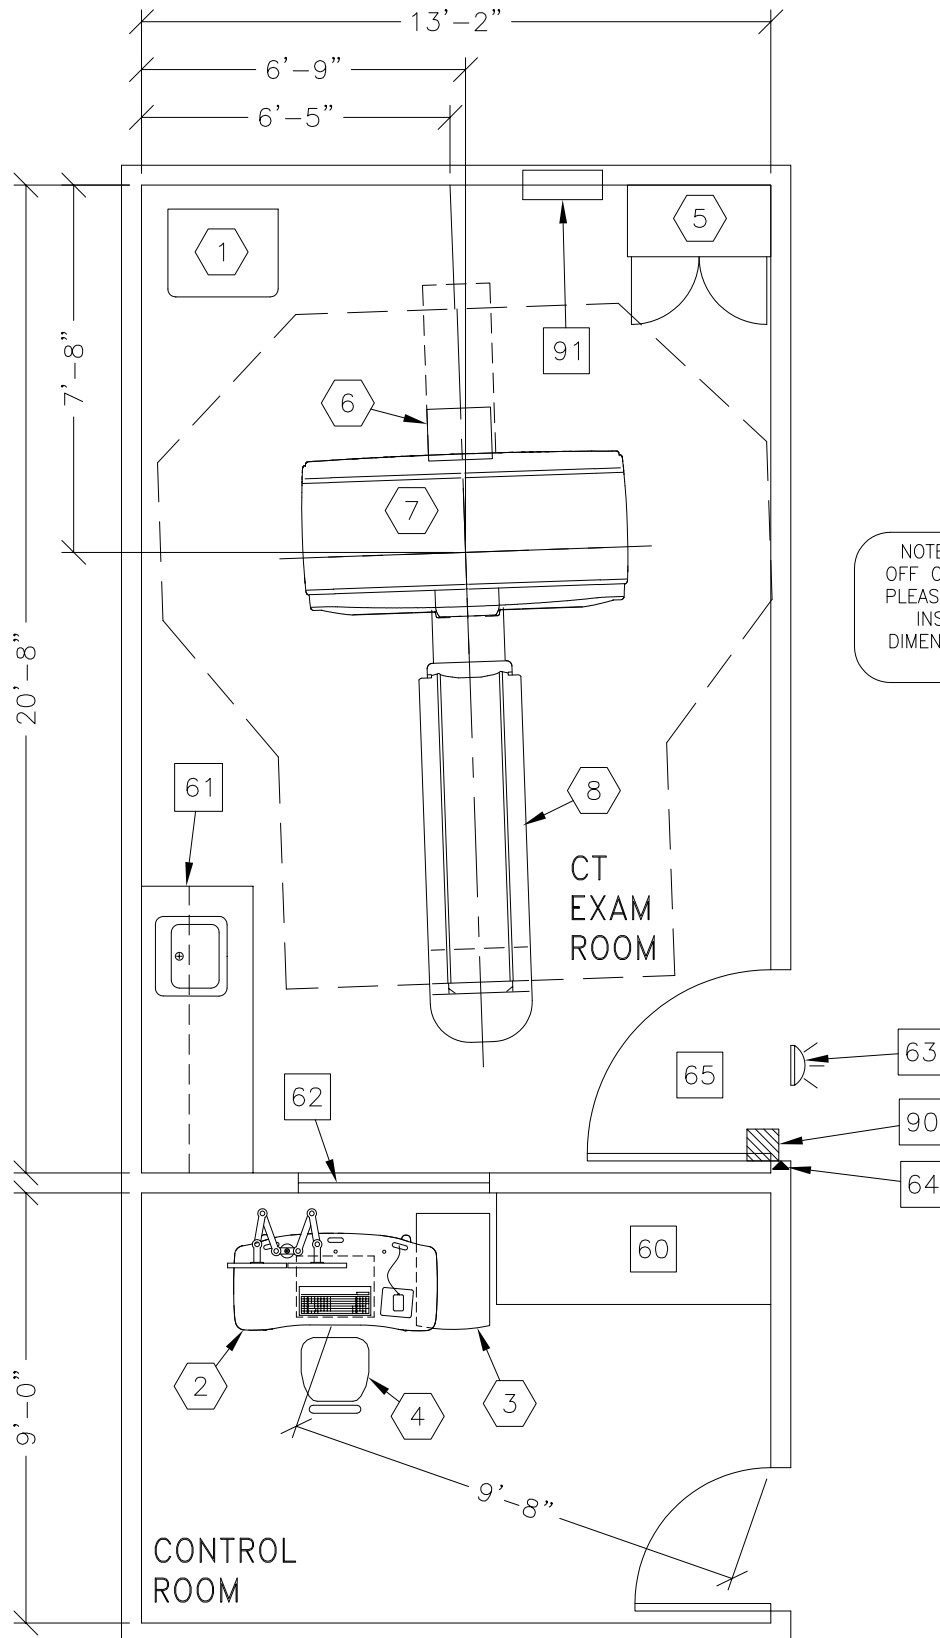

NOTE: THIS IS A SUGGESTED LAYOUT BASED OFF OF GE HEALTHCARE PRE-INSTALL MANUAL. PLEASE CONTACT LOCAL PROJECT MANAGER OF INSTALLATION IF YOUR ROOM LAYOUT OR DIMENSIONS ARE DIFFERENT THAN THE LAYOUT SHOWN.

ROOM DIMENSIONS	LENGTH & WIDTH	CEILING HEIGHT
TYPICAL:	20'-8" x 13'-2" [6.28M x 4.01M]	9'-0" [2.74M]



SEE APPENDIX "A" FOR POWER SPECIFICATIONS

ROOM PLAN LOCATED ON PAGE 6-78

ITEM	QUANTITY	ITEM DESCRIPTION	WEIGHT	HEAT OUTPUT
①	1	POWER DISTRIBUTION UNIT	816 lbs	3400 btu
②	1	FREEDOM WORKSPACE SMALL TABLE	97 lbs	
③	1	CONSOLE CABINET & LCD MONITORS	216 lbs	3200 btu
④	1	OPERATOR'S CHAIR		
⑤	1	STORAGE CABINET (EMPTY CABINET WEIGHT)	90 lbs	
⑥	1	REAR CABLE COVER		
⑦	1	CT OPTIMA CT660 GANTRY	3990 lbs	18703 btu
⑧	1	GT1700 PATIENT TABLE WITH EXTENDED TABLE TOP.	1559 lbs	1030 btu
***** CUSTOMER/CONTRACTOR SUPPLIED AND INSTALLED ITEMS *****				
60		COUNTER TOP FOR EQUIPMENT- PROVIDE GROMMETED OPENINGS AS REQUIRED TO ROUTE INTERCONNECT CABLES TO RACEWAY BELOW COUNTERTOP.		
61		COUNTER TOP WITH SINK, BASE AND WALL CABINETS		
62		LEAD GLASS WINDOW		
63		X-RAY ON WARNING LIGHT - AVAILABLE CALL: 800-200-9760 FROM GE SUPPLY GE CAT. NO. WXIABW-OF-XIU		
64		DOOR LIMIT SWITCH (REQUIRED IN SOUTH CAROLINA, OTHERWISE NEEDED ONLY IF REQUIRED BY STATE/LOCAL CODES)		
65		MINIMUM DOOR OPENING FOR EQUIPMENT DELIVERY IS 44 IN. W x 83 IN. H [1118mm x 2108mm], CONTINGENT ON A 96 IN. [2438mm] CORRIDOR WIDTH		
90		X-RAY ROOM WARNING LIGHT CONTROL PANEL REFERENCE JUNCTION POINT ' ' WLC' ON SHEET 'E1 FOR DETAILED DESCRIPTION -E4502RL FOR WARNING LIGHT CONTROL ONLY.		
91		MAIN DISCONNECT CONTROL GEMS CAT. NO. E4502AB 90 lbs., SEE DETAIL R4502AD. (IF A UPS IS NOT OR WILL NOT BE ORDERED, THE E4502AD CAN BE USED.)		

ENVIRONMENT

Ambient Operation Temperature: 64-79° (F)
 Allowable Temperature Change: 5° F [3° C] per hour
 Humidity: 30-60 percent non condensing
 Allowable Humidity Change: 5 percent per hour
 Max - Altitude: 7875 [2400M] ft. above sea level